

The Zenith Dissection Endovascular System is a line extension to the Zenith family of endovascular devices. The Dissection Endovascular Graft is similar to other endovascular grafts in the product line, but is designed specifically for treatment of dissections, having no barbs. Information from previous clinical studies and clinical use of the Zenith endovascular grafts provides a foundation for the expected clinical performance of the Dissection Endovascular Graft, including placement in aneurysmal aortic segments.

The clinical study of the Zenith Dissection Endovascular System enrolled patients with acute, complicated dissections and included implantation of the Dissection Endovascular Graft and the Dissection Stent.

Data from the clinical study performed on use of Zenith Dissection Endovascular System for the treatment of acute, complicated Type B aortic dissection are presented below.

A. Study Design

Patients were treated between August 4, 2012 and January 15, 2015. The clinical study results presented herein reflect data collected through 5-year follow-up completion on January 27, 2020. A total of 73 patients (67 US, 6 Japan) were enrolled across 22 investigational sites (21 US, 1 Japan).

This study was a prospective, nonrandomized, single-arm, multinational/multicenter clinical study based on binomial distribution for hypothesis testing.

Because acute, complicated dissections are life-threatening, the primary endpoint for the study was the survival rate at 30 days. The performance goal for this endpoint (79.4%) was an adjusted rate based on the survival rate at 30 days in the Society of Vascular Surgery (SVS) dataset, which includes pooled data from physician-sponsored studies reported by the SVS Outcomes committee.

Null Hypothesis: The survival rate at 30 days, $\pi_{s(30)}$, does not meet the performance goal (79.4%).

$$H_0: \pi_{s(30)} \leq 79.4\%$$

Alternate Hypothesis: The survival rate at 30 days, $\pi_{s(30)}$, meets the performance goal (79.4%).

$$H_A: \pi_{s(30)} > 79.4\%$$

There was an additional hypothesis-driven safety endpoint of freedom from Major Adverse Events (MAEs) at 30 days. The performance goal for this endpoint (51.2%) was an adjusted rate based on the rate of freedom from MAEs at 30 days in the SVS dataset.

Null Hypothesis: The freedom from MAE at 30 days, $\pi_{s(30)}$, does not meet the performance goal (51.2%).

$$H_0: \pi_{s(30)} \leq 51.2\%$$

Alternate Hypothesis: The freedom from MAE at 30 days, $\pi_{s(30)}$, meets the performance goal (51.2%).

$$H_A: \pi_{s(30)} > 51.2\%$$

Forty patients were necessary to assess the primary hypothesis, under an expected 30-day survival rate of 94.9% (estimated from a feasibility study conducted under G070123 for a previous design of the dissection graft and stent), with a one-sided exact binomial test, at a type I error rate of 0.025 and a power of 0.8.

Sixty patients were necessary to assess the additional hypothesis-driven endpoint, under an expected rate of freedom from 30-day MAE at 69.2% (estimated from a feasibility study conducted under G070123 for a previous design of the dissection graft and stent), with a one-sided exact binomial test, at a type I error rate of 0.025 and a power of 0.8.

A sample size of 67 was initially established to account for possible loss to follow-up. During the course of the study, the sample size was increased to 73 patients in order to account for six previously enrolled US patients who should have been excluded from the study according to additional medical exclusion criteria that were implemented subsequent to enrollment initiation (none of the six had confirmed absence of bowel necrosis at the time of enrollment). While the data from all 73 patients enrolled in the study are reported (enrollment IDs for the six excluded patients are italicized and indicated by footnotes where applicable), the hypotheses were assessed based on the 67 patients enrolled according to the inclusion/exclusion criteria.

All other endpoints were analyzed descriptively.

Even though the endpoints are at 30-days, data through 12-month post-procedure was required and has been provided on all surviving patients. This provides information on the ability of the Dissection Endovascular Graft to seal entry tears covered by the device and the ability of the Dissection Stent to provide support to delaminated segments of aortic dissections distal to the Dissection Endovascular Graft.

An independent core laboratory analyzed all patient imaging. An independent clinical events committee (CEC) adjudicated at a minimum all patient deaths, conversions to

open repair, rupture, Type A dissections, and stroke. An independent data safety monitoring board (DSMB) monitored the clinical trial according to an established safety monitoring plan.

1. Clinical Inclusion and Exclusion Criteria

Enrollment in the study was limited to patients who had an acute, complicated, Type B aortic dissection with at least one of the following characteristics:

- Aortic rupture; or
- Branch vessel obstruction/compromise resulting in malperfusion

Patients were not permitted to enroll in the study if they met any of the following exclusion criteria:

General Exclusion Criteria

- Age < 18 years (< 20 years for Japan);
- Other medical condition (e.g., cancer, congestive heart failure) that may cause the patient to be noncompliant with the Clinical Investigation Plan, confound the results, or is associated with limited life expectancy (i.e., less than 2 years);
- Pregnant, breast-feeding, or planning on becoming pregnant within 60 months;
- Unwilling or unable to comply with the follow-up schedule;
- Inability or refusal to give informed consent; or
- Simultaneously participating in another investigative device or drug study. (The patient must have completed the primary endpoint of any previous study at least 30 days prior to enrollment in this study.)

Medical Exclusion Criteria

- Suspicion of bowel necrosis (as determined by the implanting physician based on imaging observations, peritoneal signs, surgical exploration, elevated serum lactate levels, and/or acidosis)
- American Society of Anesthesiologist (ASA) risk class V (i.e., moribund patient not expected to live 24 hours with or without operation)
- Embolic stroke within the last 14 days prior to potential enrollment in the study or hemorrhagic stroke within 30 days prior to potential enrollment in the study;

- Diagnosed or suspected congenital degenerative connective tissue disease (e.g., no Marfan's or Ehler-Danlos syndrome);
- Systemic infection (e.g., sepsis);
- Bleeding diathesis, uncorrectable coagulopathy, or refuses blood transfusion;
- Allergy to stainless steel, polyester, solder (tin, silver), polypropylene, nitinol, or gold;
- Untreatable reaction to contrast, which, in the opinion of the investigator, cannot be adequately pre-medicated;
- Surgical or endovascular abdominal aortic aneurysm (AAA) repair within 30 days before or after dissection repair;
- Previous placement of a thoracic endovascular graft;
- Prior open repair involving descending thoracic aorta including suprarenal aorta and/or arch; or
- Interventional and/or open surgical procedures (unrelated to dissection) within 30 days before or after dissection repair.

Anatomical Exclusion Criteria

- Dissection of aorta proximal to left subclavian artery (either primary entry tear or most proximal extent of dissection);
- Proximal stent-graft component:
 - Aortic arch radius of curvature < 35 mm (if device deployed in the arch);
 - Proximal landing zone length measuring < 20 mm between the left common carotid artery and most proximal extent of dissection (covering left subclavian artery is acceptable, except in patients with a dominant vertebral artery off of the arch in the region of the subclavian or a dominant vertebral off of the subclavian);
 - Proximal landing zone diameter for proximal stent-graft component < 20 mm or > 38 mm, measured outer-wall to outer-wall on a sectional image or multiplanar reconstruction;
 - Distal landing zone diameter for proximal stent-graft component < 20 mm (estimate based on transaortic diameter) or > 38 mm (estimate based on true lumen diameter), measured outer-wall to outer-wall on a sectional image or multiplanar reconstruction;

- Prohibitive calcification, occlusive disease, or angulation in intended proximal landing zone;
 - Circumferential thrombus in region of intended proximal landing zone;
 - Inability to preserve the native left common carotid artery and celiac artery origins;
- Distal bare stent component:
 - Diameter < 20 mm (estimate based on transaortic diameter) or > 38 mm (estimate based on true lumen diameter) for any segment of vessel into which deployment of bare stent device is intended, measured outer-wall to outer-wall on a sectional image or multiplanar reconstruction;
 - Prohibitive angulation in segments of vessel into which deployment of bare stent device is intended (e.g., radius of curvature < 35 mm, or localized angle > 45 degrees);
- Both iliac arteries having prohibitive tortuosity, calcification, occlusive disease or arterial diameter, measured inner-wall to inner-wall on a sectional image, that are not conducive to placement of the introducer sheath (use of access conduit permitted); or
- Aneurysm or angulation in the distal thoracic aorta that would preclude advancement of the introduction system.

2. Follow-up Schedule

All patients were scheduled to return for follow-up examinations at 30 days, 6 months, 12 months, and then annually through 5 years postoperatively.

Preoperatively, patients underwent a clinical exam, blood test, and CT scan, as also shown in Table 1. Postoperatively, the objective parameters measured during the study based on CT included assessment of the total aortic, true lumen, and false lumen diameters at multiple locations, presence of and sources for false lumen flow, extent of false lumen thrombosis, progression of dissection, branch vessel patency, and device position and integrity. Adverse events and complications were recorded at all visits.

The key timepoints are shown below in Table 1 as well as the tables that follow summarizing safety and effectiveness.

Table 1. Study follow-up schedule

	Pre-operative	Intra-operative	Post-procedure	30-day (± 10 days)	6-month (± 30 days)	12-month (± 45 days)	2-year to 5-year^e
Clinical exam	X		X	X	X	X	X
Blood tests ^a	X		X	X	X	X	X ^f
Contrast CT scan	X		X ^{c,d}		X ^c	X ^c	X ^c
Angiography	X ^b	X					

^a Including tests to evaluate kidney and liver function.

^b Required only to resolve any uncertainties in anatomical measurements necessary for graft sizing.

^c Transesophageal echocardiography (TEE) or non-contrast CT imaging may be used for those patients experiencing documented renal failure (eGFR < 30) or who are otherwise unable to undergo contrast enhanced CT scan.

^d CT must be performed prior to hospital discharge. In case of impaired renal function at the time of discharge, CT may be performed at 30 days.

^e 2 years (730 ± 60 days), 3 years (1095 ± 60 days), 4 years (1460 ± 90 days), and 5 years (1825 ± 90 days).

^f Required only for patients with malperfusion that has not stabilized.

3. Clinical Endpoints

With regards to safety and effectiveness, the primary endpoint is the survival rate at 30 days.

With regards to safety, an additional hypothesis-driven endpoint for the study was freedom from major adverse events (MAEs) at 30 days. MAEs were defined as the following: myocardial infarction, chronic renal insufficiency/chronic renal failure requiring dialysis, bowel ischemia, stroke, paraplegia or paraparesis, and prolonged (> 72 hours) ventilatory support.

With regards to success/failure criteria, the study would be considered successful if both performance goals were met.

Additional (secondary) endpoints that were evaluated, not for the purpose of statistical inference, included changes in aortic, true and false lumen size, presence of and sources for false lumen flow, extent of false lumen thrombosis, progression of dissection, branch vessel patency, secondary interventions, and device migration and integrity.

B. Accountability of PMA Cohort (Through 12 Months)

At the time of the database lock for the PMA (March 14, 2017), of 73 patients enrolled in the PMA study, 94.5% (69) were available for 30-day follow-up and 78.1% (57) were available for 12-month follow-up, as there were 4 deaths within 30 days and 9 deaths as well as 3 patients who withdrew from the study or became lost to follow-up between the 30-day and 12-month visits; these 12-month follow-up availability results were

unchanged through completion of 5-year follow-up. Table 2 reports the follow-up availability through 12 months.

Of the 73 patients enrolled in the study, 79.5% (58) received at least one Dissection Endovascular Graft and one Dissection Stent during the index procedure, while the remaining 20.5% (15) received only a Dissection Endovascular Graft, not a Dissection Stent. Although the study was not powered to assess for differences in outcomes based on the different component combinations (namely the presence vs. absence of a Dissection Stent), the results were analyzed and reported separately for the following groups where appropriate: total patient population, cohort with a Dissection Stent, and cohort without a Dissection Stent.

Table 2. Follow-up availability

Follow-up Visit ^c	Patients Eligible for Follow-up	Percent of Data Available (Site)		Adequate Imaging to Assess the Parameter (Core Laboratory)						Events Occurring Before Next Interval			
		Clinical Assessment	CT ^a	Size Increase in Stent-graft	Size Increase in Dissection Stent ^b	Entry-flow in Thoracic Aorta	Entry-flow in Abdominal Aorta	Migration	Device Integrity	Death	Conversion	LTF/ WTHD	Not Due for Next Visit
Postoperative	73	100.0% (73/73)	53.4% (39/73)	NA	NA	45.2% (33/73)	45.2% (33/73)	NA	49.3% (36/73)	4	0	0	0
30-day	69	97.1% (67/69)	76.8% (53/69)	NA	NA	71.0% (49/69)	68.1% (47/69)	NA	75.4% (52/69)	1	0	1	0
6-month	67	77.6% (52/67)	83.6% (56/67)	98.2% (55/67)	84.6% (44/52)	76.1% (51/67)	70.1% (47/67)	74.6% (50/67)	83.6% (56/67)	8	0	2	0
12-month	57	86.0% (49/57)	89.5% (51/57)	92.2% (47/57)	84.8% (39/46)	82.5% (47/57)	78.9% (45/57)	80.7% (46/57)	86.0% (49/57)	2	1	5	0

LTF: lost-to-follow-up; WTHD: withdrawal.

^a Per clinical investigation plan amendment 11-007-04, a patient is required to have a CT scan prior to discharge unless the patient has renal issues; in this case, the patient will have the CT scan completed at the 1-month visit.^b Size increase in Dissection Stent assessment only applies to patients who received a Dissection Stent.^c Follow-up visit windows as follows: 30 days (± 10 days), 6 months (180 ± 30 days), 12 months (365 ± 45 days).

C. Study Population Demographics and Baseline Parameters

The demographics and baseline parameters of the study population are typical for an acute, complicated Type B aortic dissection study performed in the US.

The demographics, pre-existing comorbid medical conditions, and presenting complications were compared between this study and SVS dataset to support the use of the performance goals based on the SVS dataset. Comparisons were also made between two patient groups within the study; patients who received and patients who did not receive a Dissection Stent.

Partially due to the small number of patients, few statistically significant differences were found when comparing populations, despite numerical differences. None of the differences were found to be clinically meaningful with respect to supporting the performance goals. Some of the differences in the patient groups within the study population are likely associated with the greater percentage of patients who did not receive the Dissection Stent having been treated for rupture rather than malperfusion.

Comparisons are not presented between the US and Japanese patients as only 6 patients were treated in Japan. Four patients presented with rupture, one patient presented with rupture and malperfusion, and one patient presented with malperfusion alone; none received the Dissection Stent.

Demographics

The demographics and patient characteristics are presented in Table 3. Of the demographic and patient data in the present study compared with that of the SVS dataset, only the ethnicity/race distribution was significantly different ($p = 0.046$), which is not expected to be clinically significant with respect to evaluating the safety and effectiveness endpoints. Similarly, with the exception of the ethnicity distribution, the demographics appeared comparable between patients who either received or did not receive a Dissection Stent.

Table 3. Demographics and patient characteristics

Demographic	Mean $\pm$ SD (N, range) or Percent Patients (number/total number)			
	Without Dissection Stent	With Dissection Stent	All Pivotal Patients	SVS Acute Patients
Age (years) All patients	65.1 $\pm$ 13.1 (15, 42 - 81)	59.5 $\pm$ 10.1 (58, 34 - 77)	60.7 $\pm$ 10.9 (73, 34 - 81)	58.8 $\pm$ 15.4 (85, 25.9 - 88.6)

Demographic	Mean ± SD (N, range) or Percent Patients (number/total number)			
	Without Dissection Stent	With Dissection Stent	All Pivotal Patients	SVS Acute Patients
Gender				
Male	53.3% (8/15)	69.0% (40/58)	65.8% (48/73)	72.9% (62/85)
Female	46.7% (7/15)	31.0% (18/58)	34.2% (25/73)	27.1% (23/85)
Ethnicity/Race ^a				
White	33.3% (5/15)	67.2% (39/58)	60.3% (44/73)	52.9% (45/85)
Hispanic or Latino	0%	5.2% (3/58)	4.1% (3/73)	14.1% (12/85)
Black or African American	20.0% (3/15)	25.9% (15/58)	24.7% (18/73)	27.1% (23/85)
First Nations ^b	0%	0%	0%	2.4% (2/85)
Asian	46.7% (7/15)	1.7% (1/58)	11.0% (8/73)	3.5% (3/85)
Height (in)	64.4 ± 3.6 (15, 59.8 - 72.0)	68.5 ± 4.4 (58, 59 - 76)	67.7 ± 4.5 (73, 59 - 76)	NC
Weight (lbs)	167.8 ± 38.9 (15, 116.0 - 255.2)	202.5 ± 55.9 (58, 101.2 - 356.4)	195.1 ± 54.4 (73, 101.2 - 356.4)	NC
Body mass index (BMI)	28.4 ± 5.5 (15, 21.4 - 40.0)	30.0 ± 7.2 (57, 16.3 - 50.6)	29.7 ± 6.9 (72, 16.3 - 50.6)	NC

NC: not collected.

^a Ethnicity/race distribution difference was significant between the pivotal study and SVS dataset ($p = 0.046$).

^b First Nations includes American Indian/Alaskan Native, and Native Hawaiian/Pacific Islander.

Medical History and Comorbidities

Medical history and comorbid conditions are presented in Table 4. None of the differences in the medical histories of patients enrolled in the present study and those recorded in the SVS dataset are statistically significant. A history of aneurysm or dissection is the biggest difference in patient groups within the study, being more prevalent in patients that did not receive a Dissection Stent.

Table 4. Medical history and comorbid conditions

Medical History	Percent Patients (number/total number)			
	Without Dissection Stent	With Dissection Stent	All Pivotal Patients	SVS Acute Patients
Cardiovascular				
Previous myocardial infarction	13.3% (2/15)	3.4% (2/58)	5.5% (4/73)	11.8% (10/85)
Previous symptomatic congestive heart failure	0% (0/15)	3.4% (2/58)	2.7% (2/73)	10.6% (9/85)
Coronary artery disease	20.0% (3/15)	15.5% (9/58)	16.4% (12/73)	NC
Cardiac arrhythmia	20.0% (3/15)	13.8% (8/58)	15.1% (11/73)	11.8% (10/85)

Medical History	Percent Patients (number/total number)			
	Without Dissection Stent	With Dissection Stent	All Pivotal Patients	SVS Acute Patients
Vascular				
Thromboembolic event	0%	8.6% (5/58)	6.8% (5/73)	NC
Peripheral vascular disease	6.7% (1/15)	3.4% (2/58)	4.1% (3/73)	2.4% (2/85)
Family history of aneurysm or dissection	0%	6.9% (4/58)	5.5% (4/73)	NC
Patient history of aneurysm or dissection	60.0% (9/15)	22.4% (13/58)	30.1% (22/73)	NC
Hypertension	100.0% (15/15)	82.8% (48/58)	86.3% (63/73)	83.5% (71/85)
Previous thoracic surgery or thoracic trauma	26.7% (4/15)	10.3% (6/58)	13.7% (10/73)	NC
Aortobronchial fistula	0%	0%	0%	NC
Aortoesophageal fistula	0%	0%	0%	NC
Bleeding diathesis or uncorrectable coagulopathy	0%	0%	0%	NC
Carotid endarterectomy	0%	0%	0%	NC
Diagnosed or suspected congenital degenerative collagen disease	0%	0%	0%	NC
Pulmonary				
Chronic obstructive pulmonary disease	40.0% (6/15)	15.5% (9/58)	20.5% (15/73)	10.6% (9/85)
Renal				
Chronic renal insufficiency or dialysis	6.7% (1/15)	8.6% (5/58)	8.2% (6/73)	7.1% (6/85)
Endocrine				
Diabetes	0%	5.2% (3/58)	4.1% (3/73)	12.9% (11/85)
Infectious disease				
Previous diagnosis of sepsis	0%	0%	0%	NC
Hepatobiliary				
Liver disease	6.7% (1/15)	1.7% (1/58)	2.7% (2/73)	0% (0/85)
Neoplasms				
Cancer	20.0% (3/15)	8.6% (5/58)	11.0% (8/73)	9.4% (8/85)
Neurologic				
Stroke	13.3% (2/15)	5.2% (3/58)	6.8% (5/73)	NC
Paraparesis	6.7% (1/15)	5.2% (3/58)	5.5% (4/73)	1.2% (1/85)
Paralysis	0%	3.4% (2/58)	2.7% (2/73)	2.4% (2/85)
Transient ischemic attack	6.7% (1/15)	3.4% (2/58)	4.1% (3/73)	0% (0/85)
Smoking				
Past	13.3% (2/15)	31.0% (18/58)	27.4% (20/73)	37.3% (31/83)
Current	40.0% (6/15)	50.0% (29/58)	47.9% (35/73)	32.5% (27/83)
Never	46.7% (7/15)	19.0% (11/58)	24.7% (18/73)	30.1% (25/83)

NC: not collected.

ASA Classification

Table 5 reports the ASA classification. The distribution of ASA physical status classifications in the present study was statistically different from that in the SVS dataset, with the SVS patients having more severe disease. However, due to the subjective nature of the ASA classification, and considering the similarities between the present study and

the SVS dataset for most other variables, the difference is not considered clinically significant with respect to establishing the performance goals. The majority of patients were class 4 in both the group with a Dissection Stent and group without a Dissection Stent.

Table 5. ASA physical status classification

ASA Classification ^a	Percent Patients (number/total number)			
	Without Dissection Stent	With Dissection Stent	Total	SVS
Healthy patient (1)	0%	0%	0%	0%
Mild systemic disease (2)	20.0% (3/15)	5.2% (3/58)	8.2% (6/73)	2.4% (2/85)
Severe systemic disease (3)	20.0% (3/15)	29.3% (17/58)	27.4% (20/73)	22.4% (19/85)
Incapacitating systemic disease (4)	60.0% (9/15)	65.5% (38/58)	64.4% (47/73)	64.7% (55/85)
Moribund patient (5)	0%	0%	0%	10.6% (9/85)

^a ASA classification distribution difference was significant between the present study and the SVS dataset ($p = 0.008$).

SVS-ISCVS Risk Score

Table 6 reports the Society for Vascular Surgery/International Society for Cardiovascular Surgery (SVS-ISCVS) risk score. The SVS-ISCVS risk scores were consistent with the preexisting comorbid conditions for the patient population in the present study. Of the distribution of risk scores, patients who received a Dissection Stent were more likely to present with higher smoking risk scores and higher renal status risk scores, leading to higher total risk scores. SVS-ISCVS risk scores were not reported in the SVS dataset.

Table 6. SVS-ISCVS risk score classification

SVS-ISCVS Category	Percent Patients (number/total number)		
	Without Dissection Stent	With Dissection Stent	Total
Diabetes risk score			
0	100.0% (15/15)	93.1% (54/58)	94.5% (69/73)
1	0%	5.2% (3/58)	4.1% (3/73)
2	0%	0%	0%
3	0%	1.7% (1/58)	1.4% (1/73)
4	0%	0%	0%
Smoking risk score			
0	53.3% (8/15)	34.5% (20/58)	38.4% (28/73)
1	6.7% (1/15)	12.1% (7/58)	11.0% (8/73)
2	33.3% (5/15)	32.8% (19/58)	32.9% (24/73)
3	6.7% (1/15)	20.7% (12/58)	17.8% (13/73)

SVS-ISCVS Category	Percent Patients (number/total number)		
	Without Dissection Stent	With Dissection Stent	Total
Hypertension risk score			
0	6.7% (1/15)	13.8% (8/58)	12.3% (9/73)
1	33.3% (5/15)	20.7% (12/58)	23.3% (17/73)
2	20.0% (3/15)	32.8% (19/58)	30.1% (22/73)
3	40.0% (6/15)	32.8% (19/58)	34.2% (25/73)
Hyperlipidemia risk score			
0	53.3% (8/15)	56.9% (33/58)	56.2% (41/73)
1	13.3% (2/15)	12.1% (7/58)	12.3% (9/73)
2	0%	1.7% (1/58)	1.4% (1/73)
3	33.3% (5/15)	29.3% (17/58)	30.1% (22/73)
Cardiac status risk score			
0	86.7% (13/15)	89.7% (52/58)	89.0% (65/73)
1	13.3% (2/15)	1.7% (1/58)	4.1% (3/73)
2	0%	6.9% (4/58)	5.5% (4/73)
3	0%	1.7% (1/58)	1.4% (1/73)
Carotid disease risk score			
0	93.3% (14/15)	94.8% (55/58)	94.5% (69/73)
1	6.7% (1/15)	3.4% (2/58)	4.1% (3/73)
2	0%	0%	0% (0/73)
3	0%	1.7% (1/58)	1.4% (1/73)
Renal status risk score			
0	93.3% (14/15)	62.1% (36/58)	68.5% (50/73)
1	6.7% (1/15)	31.0% (18/58)	26.0% (19/73)
2	0%	5.2% (3/58)	4.1% (3/73)
3	0%	1.7% (1/58)	1.4% (1/73)
Pulmonary status risk score			
0	80.0% (12/15)	73.7% (42/57)	75.0% (54/72)
1	6.7% (1/15)	17.5% (10/57)	15.3% (11/72)
2	0%	5.3% (3/57)	4.2% (3/72)
3	13.3% (2/15)	3.5% (2/57)	5.6% (4/72)
Total SVS-ISCVS risk score (mean ± SD; N, range)	4.7 ± 2.4 (15, 1 - 9)	5.5 ± 2.9 (58, 0 - 12)	5.4 ± 2.8 (73, 0 - 12)

Presenting Complications

Presenting complications reported by the site are presented in Table 7. The percentage of patients with rupture, malperfusion, or rupture and malperfusion were comparable between the present study and the SVS dataset, though the patient population in the present study significantly more often presented with obstruction/compromise that also involved the gastrointestinal ($p < 0.001$) and renal/urologic branch vessels ($p = 0.011$). Patients who presented with rupture were less likely to receive a Dissection Stent than patients who presented with obstruction or compromise.

Table 7. Presenting complications

Complication	Percent Patients (number/total number)			
	Without Dissection Stent	With Dissection Stent	Total	SVS
Rupture	73.3% (11/15)	15.5% (9/58)	27.4% (20/73)	31.8% (27/85)
Obstruction/compromise of branch vessel	33.3% (5/15)	89.7% (52/58)	78.1% (57/73)	71.8% (61/85)
Gastrointestinal	40.0% (2/5)	59.6% (31/52)	57.9% (33/57) ^a	19.7% (12/61) ^a
Renal/urologic	60.0% (3/5)	57.7% (30/52)	57.9% (33/57) ^a	36.1% (22/61) ^a
Spinal cord	0%	5.8% (3/52)	5.3% (3/57)	3.3% (2/61)
Lower extremity	80.0% (4/5)	53.8% (28/52)	56.1% (32/57)	55.7% (34/61)
Other	0%	1.9% (1/52)	1.8% (1/57)	8.2% (5/61)
Rupture and obstruction of branch vessel	6.7% (1/15)	5.2% (3/58)	5.5% (4/73)	3.5% (3/85)
Persistent pain	93.3% (14/15)	91.4% (53/58)	91.8% (67/73) ^a	76.5% (65/85) ^a
Size/growth of the transaortic diameter	53.3% (8/15)	15.5% (9/58)	23.3% (17/73)	NC
Periaortic effusion (without rupture)	60.0% (9/15)	12.1% (7/58)	21.9% (16/73)	NC
Resistant hypertension	40.0% (6/15)	27.6% (16/58)	30.1% (22/73)	43.5% (37/85)

NC: not collected.

^a Persistent pain, gastrointestinal, and renal/urologic obstruction/compromise of branch vessel distribution differences were significant between the present study and the SVS dataset ($p = 0.010$, $p < 0.001$, and $p = 0.011$, respectively).

Baseline Vessel Measurements

This section reports the results from core laboratory analysis of pre-procedure imaging.

Site vs Core Laboratory Measures

Imaging was reviewed by the clinical study sites to determine adherence to the study selection criteria. All patients enrolled in the study were reported by the sites to meet the selection criteria. However, a total of 33 patients were measured by the core laboratory as having a length < 20 mm from the left common carotid (LCC) to the most proximal extent of dissection (Table 8), 25 of whom also had a dissection that extended proximal to the left subclavian artery (LSA) according to initial assessments relative to anatomical landmarks (Table 10) or based on the Zone classification¹ as also used to describe the extent of Dissection Endovascular Graft and Dissection Stent coverage at the time of the index procedure (Table 18, found in the Procedural Information Section). There were 11 additional patients (in whom the length from LCC to proximal extent was either not assessed or measured ≥ 20 mm by core laboratory) with a dissection that extended proximal the LSA based on the Zone classification. Refer to Figure 1 for an overview of these findings.

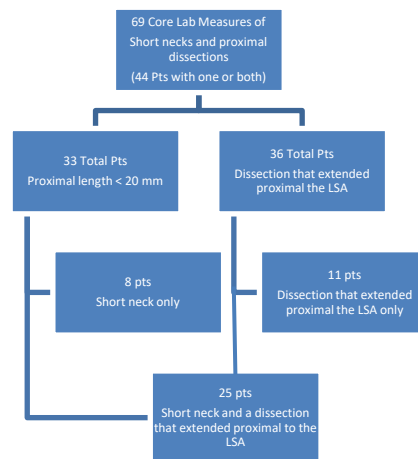


Figure 1. Core laboratory measurements of short necks and/or dissection proximal to the LSA

Also of note, the maximum total aortic diameters (Table 8) in locations expected to coincide with likely fixation/seal zones (i.e., just distal to the LCC and just distal to the LSA) exceeded the maximum allowable diameter of 38 mm at pre-procedure (n=14, which included 12 of the patients with a length < 20 mm from the LCC to proximal extent of dissection and/or a dissection that extended proximal to the LSA).

While patients were to be excluded from the study if the length from the LCC to the most proximal extent of dissection was < 20 mm, if the dissection extended proximal to the LSA, or if the total aortic diameter was > 38 mm in the proximal fixation zone, compliance with the protocol was based on information available at pre-procedure, as assessed by the site, and not the results from subsequent core laboratory analysis of pre-procedure imaging. All site assessments concurred with the requirements in the protocol. Nonetheless, it is important to note that all proximal post-treatment dissection events (4/4), ruptures (2/2), and proximal Type I entry-flow (7/7) within 365 days occurred in this subset of patients with anatomy beyond the intended use, underscoring the need to pay careful attention to these parameters during patient selection, as also emphasized in the labeling.

Length and Diameter

Table 8 reports baseline anatomical measurements per the core laboratory (similar data were not reported in the SVS dataset). The overall results from core laboratory analysis of pre-procedure imaging appear consistent with expectations for the intended study patient population, and the majority of the anatomical measurements for patients who

received a Dissection Stent and for those who did not appeared comparable, with the exception of some diameters and lengths, as follows.

With regards to length, patients who did not receive a Dissection Stent (patients who often presented with aortic rupture) typically exhibited more focal dissections (i.e., shorter length of dissected aorta) when compared to patients who received a Dissection Stent (patients who often presented with obstruction/compromise of branch vessels). Additionally, the average length of dissection (408.9 mm) in patients who received a Dissection Stent approached the total length of aorta from the left common carotid artery to the aortic bifurcation, thus indicating near complete involvement of the aorta with dissection. Overall, the trends in length were not surprising given the apparent difference in presenting complications between groups.

With regards to diameter, patients who did not receive a Dissection Stent were more likely to have presented with larger transaortic diameters in the descending thoracic aorta, which is not surprising considering these patients were more often treated for rupture when compared to the patients who received a Dissection Stent. Patients who received a Dissection Stent were more likely to display larger false lumen diameters in the aorta distal to the descending thoracic aorta, specifically within the region of the branch vessels (aorta at the level of the celiac artery, SMA, and both renal arteries) as well as in the abdominal aorta, which is also not surprising considering these patients were more often treated for malperfusion when compared to patients who did not receive a Dissection Stent.

Table 8. Baseline anatomical measurements per the core laboratory

Anatomical Measurements	Mean ± SD (N, range)		
	Without Dissection Stent	With Dissection Stent	Total
Length (mm)			
LCC to most proximal extent of dissection	26.8 ± 37.7 (13, -11.1 to 118.4)	23.9 ± 38.8 (53, -109.2 to 191.5)	24.5 ± 38.3 (66, -109.2 to 191.5)
LCC to most proximal aspect of primary tear	93.5 ± 56.8 (11, 5.9 - 208.8)	112.2 ± 69.4 (48, 0.9 - 281.7)	108.7 ± 67.2 (59, 0.9 - 281.7)
From most proximal to most distal aspect of dissection	315.9 ± 100.1 (13, 129.3 - 468.9)	408.9 ± 121.3 (40, 125.2 - 637.2)	386.1 ± 122.4 (53, 125.2 - 637.2)
Aortic arch radius of curvature (mm)	26.6 ± 4.9 (15, 19 - 40)	28.2 ± 7.0 (56, 13 - 47)	27.8 ± 6.6 (71, 13 - 47)
Largest angle in the descending thoracic aorta (degrees)	32.7 ± 27.1 (14, 0 - 99)	31.1 ± 26.6 (55, 0 - 175)	31.4 ± 26.5 (69, 0 - 175)

Anatomical Measurements	Mean ± SD (N, range)		
	Without Dissection Stent	With Dissection Stent	Total
Maximum aortic diameter (mm)			
Just distal to LCC origin			
True lumen	33.3 ± 3.6 (15, 26.3 - 40.5)	32.4 ± 4.3 (56, 16.3 - 43.8)	32.6 ± 4.2 (71, 16.3 - 43.8)
False lumen	0.4 ± 1.5 (15, 0 - 5.7)	0.6 ± 2.6 (56, 0 - 16.1)	0.6 ± 2.4 (71, 0 - 16.1)
Total	33.6 ± 3.4 (15, 26.3 - 40.5)	33.1 ± 4.1 (56, 25.7 - 43.8)	33.2 ± 3.9 (71, 25.7 - 43.8)
Just distal to LSA origin			
True lumen	27.8 ± 6.8 (15, 12.5 - 35.7)	27.7 ± 4.4 (56, 18.2 - 40.3)	27.7 ± 5.0 (71, 12.5 - 40.3)
False lumen	6.1 ± 8.8 (15, 0 - 26.7)	4.4 ± 4.9 (56, 0 - 17.9)	4.8 ± 5.9 (71, 0 - 26.7)
Total	33.9 ± 6.2 (15, 26.4 - 51.1)	32.1 ± 4.5 (56, 24.3 - 43.3)	32.5 ± 4.9 (71, 24.3 - 51.1)
Descending thoracic aorta			
True lumen	25.4 ± 12.9 (15, 4.0 - 44.6)	21.5 ± 10.0 (56, 6.2 - 65.9)	22.3 ± 10.7 (71, 4.0 - 65.9)
False lumen	19.2 ± 12.0 (15, 0 - 49.8)	18.2 ± 8.0 (56, 0 - 34.1)	18.4 ± 8.9 (71, 0 - 49.8)
Total	44.6 ± 10.9 (15, 29.5 - 64.4)	39.6 ± 5.7 (56, 26.8 - 65.9)	40.7 ± 7.3 (71, 26.8 - 65.9)
Just distal to celiac artery origin			
True lumen	19.8 ± 8.7 (14, 3.6 - 32.6)	14.3 ± 6.5 (55, 3.4 - 28.4)	15.5 ± 7.2 (69, 3.4 - 32.6)
False lumen	10.0 ± 12.6 (14, 0 - 43.4)	14.3 ± 6.4 (55, 0 - 28.1)	13.4 ± 8.1 (69, 0 - 43.4)
Total	29.8 ± 8.6 (14, 21.9 - 55.3)	28.6 ± 3.4 (55, 19.5 - 39.4)	28.9 ± 4.9 (69, 19.5 - 55.3)
Just distal to SMA origin			
True lumen	19.2 ± 8.5 (14, 2.6 - 30.2)	15.0 ± 6.6 (53, 2.1 - 26.9)	15.8 ± 7.2 (67, 2.1 - 30.2)
False lumen	7.4 ± 10.0 (14, 0 - 29.0)	12.2 ± 7.6 (53, 0 - 27.8)	11.2 ± 8.3 (67, 0 - 29.0)
Total	26.6 ± 5.2 (14, 20.4 - 42.3)	27.1 ± 3.7 (53, 20.0 - 37.9)	27.0 ± 4.1 (67, 20.0 - 42.3)
Just distal to right renal artery origin			
True lumen	17.4 ± 7.2 (14, 3.1 - 26.1)	14.9 ± 6.1 (52, 2.7 - 26.9)	15.4 ± 6.3 (66, 2.7 - 26.9)
False lumen	5.7 ± 7.6 (14, 0 - 20.1)	9.7 ± 6.9 (52, 0 - 29.2)	8.9 ± 7.2 (66, 0 - 29.2)
Total	23.2 ± 4.1 (14, 17.2 - 32.0)	24.6 ± 3.7 (52, 17.2 - 37.9)	24.3 ± 3.8 (66, 17.2 - 37.9)
Just distal to left renal artery origin			
True lumen	17.4 ± 7.6 (14, 2.4 - 26.1)	14.5 ± 6.3 (53, 3.2 - 27.8)	15.1 ± 6.6 (67, 2.4 - 27.8)
False lumen	5.9 ± 8.1 (14, 0 - 20.5)	9.7 ± 8.0 (53, 0 - 36.0)	8.9 ± 8.1 (67, 0 - 36.0)
Total	23.3 ± 4.6 (14, 18.0 - 33.6)	24.2 ± 4.1 (53, 17.1 - 40.1)	24.0 ± 4.2 (67, 17.1 - 40.1)
Abdominal aorta			
True lumen	25.0 ± 12.8 (14, 7.4 - 53.0)	16.5 ± 7.7 (48, 3.8 - 36.3)	18.4 ± 9.7 (62, 3.8 - 53.0)
False lumen	12.3 ± 12.5 (14, 0 - 43.4)	16.1 ± 7.9 (48, 0 - 36.6)	15.3 ± 9.2 (62, 0 - 43.4)
Total	37.3 ± 11.6 (14, 24.1 - 55.3)	32.6 ± 4.9 (48, 24.1 - 44.8)	33.6 ± 7.2 (62, 24.1 - 55.3)

LCC: left common carotid artery; LSA: left subclavian artery; SMA: superior mesenteric artery; CIA: common iliac artery.

Location of Primary Tear

Table 9 reports the location of the primary tear as assessed by the core laboratory. As expected for a study of patients with Type B dissection, the majority of primary tears for the total patient population occurred in the descending thoracic aorta. The distribution in primary tear location appeared to be similar for both patient populations based on core laboratory analysis.

Table 9. Location of primary tear per the core laboratory

Location	Percent Patients (number/total number)		
	Without Dissection Stent	With Dissection Stent ^a	Total
Aorta at LSA/in LSA	0%	1.8% (1/57)	1.4% (1/72)
Descending thoracic aorta, distal to LSA	86.7% (13/15)	86.0% (49/57)	86.1% (62/72)
Aorta at celiac artery/in celiac artery	0%	0%	0%
Aorta at SMA/in SMA	0%	0%	0%
Aorta at renal arteries/in renal arteries	0%	0%	0%
Infrarenal abdominal aorta	0%	0%	0%
Unknown	13.3% (2/15)	12.3% (7/57)	12.5% (9/72)

LCC: left common carotid artery; LSA: left subclavian artery; SMA: superior mesenteric artery.

^a Patient 1130090 was unable to be assessed by the core laboratory due to inadequate imaging.

Location of Proximal Extent of Dissection

Table 10 provides the distribution of the location of the proximal aspect of dissection as determined by the core laboratory. The majority of the total patient population had the proximal aspect of dissection either at or distal to the LSA, while some patients were noted by the core laboratory to have a dissection with the most proximal aspect in the ascending aorta, aortic arch (proximal to the LCC), or proximal to the LSA (distal to the LCC). Likewise, the majority of patients in both groups had the proximal aspect of the dissection either at or distal to the LSA.

Table 10. Location of the proximal aspect of dissection as determined by the core laboratory

Location	Percent Patients (number/total number)		
	Without Dissection Stent	With Dissection Stent ^a	Total
Ascending thoracic aorta	0%	3.5% (2/57)	2.8% (2/72)
Aortic arch, proximal to LCC	20.0% (3/15)	1.8% (1/57)	5.6% (4/72)
Proximal to LSA, distal to LCC	6.7% (1/15)	10.5% (6/57)	9.7% (7/72)
Aorta at LSA/in LSA	20.0% (3/15)	50.9% (29/57)	44.4% (32/72)
Descending thoracic aorta, distal to LSA	53.3% (8/15)	31.6% (18/57)	36.1% (26/72)
Aorta at celiac artery/in celiac artery	0%	0%	0%
Aorta at SMA/in SMA	0%	0%	0%

Location	Percent Patients (number/total number)		
	Without Dissection Stent	With Dissection Stent ^a	Total
Aorta at renal arteries	0%	0%	0%
Infrarenal abdominal aorta	0%	0%	0%
Unknown	0%	1.8% (1/57)	1.4% (1/72)

LCC: left common carotid artery; LSA: left subclavian artery; SMA: superior mesenteric artery.

^a Patient 1130090 was unable to be assessed by the core laboratory due to inadequate imaging.

Location of Distal Extent of Dissection

Table 11 provides the distribution of the location of the distal aspect of dissection as determined by the core laboratory. The dissection often extended distally to at least the level of the celiac artery, with the majority of dissections for the total patient population terminating distal to the renal arteries, in either the abdominal aorta or common/external iliac arteries. Compared to the patients who did not receive a Dissection Stent, those patients who did receive a Dissection Stent appeared to more often have a dissection that terminated in the external iliac arteries.

Table 11. Location of the most distal aspect of dissection as determined by the core laboratory

Location	Percent Patients (number/total number)		
	Without Dissection Stent ^a	With Dissection Stent ^b	Total
Aorta at celiac artery/in celiac artery	8.3% (1/12)	0%	1.5% (1/68)
Aorta at SMA/in SMA	16.7% (2/12)	3.6% (2/56)	5.9% (4/68)
Aorta at renal arteries/in renal arteries	8.3% (1/12)	12.5% (7/56)	11.8% (8/68)
Infrarenal abdominal aorta	25.0% (3/12)	19.6% (11/56)	20.6% (14/68)
Common iliac arteries (right or left)	25.0% (3/12)	17.9% (10/56)	19.1% (13/68)
External iliac arteries (right or left)	0%	28.6% (16/56)	23.5% (16/68)
Internal iliac arteries (right or left)	0%	1.8% (1/56)	1.5% (1/68)
Femoral arteries (right or left)	0%	0%	0%
Unknown	16.7% (2/12)	16.1% (9/56)	16.2% (11/68)

SMA: superior mesenteric artery.

^a Patients 1130049, 1230003, and 1230007 were unable to be assessed by the core laboratory due to inadequate imaging.

^b Patients 1130057 and 1130090 were unable to be assessed by the core laboratory due to inadequate imaging.

Secondary Tears

Table 12 provides the distribution of the location of the identified secondary/reentry tears as determined by the core laboratory. The majority of the total patient population presented with secondary tears, often in the descending thoracic aorta as well as in the abdominal aorta and at/near the renal arteries. While most patients in both groups had secondary tears in the descending thoracic aorta, it appeared that patients who received a

Dissection Stent had a higher prevalence of secondary tears in the region of the branch vessels (renal arteries, SMA, celiac artery), abdominal aorta, and iliac arteries.

Table 12. Location of the secondary/reentry tears as determined by the core laboratory^a

Location	Percent Patients (number/total number)		
	Without Dissection Stent	With Dissection Stent ^b	Total
None	13.3% (2/15)	3.5% (2/57)	5.6% (4/72)
Ascending thoracic aorta	0%	0%	0%
Aortic arch, proximal to LCC	0%	0%	0%
Proximal to LSA, distal to LCC	0%	0%	0%
Aorta at LSA/in LSA	0%	0%	0%
Descending thoracic aorta, distal to LSA	80.0% (12/15)	84.2% (48/57)	83.3% (60/72)
Aorta at celiac artery/in celiac artery	6.7% (1/15)	28.1% (16/57)	23.6% (17/72)
Aorta at SMA/in SMA	0% (0/15)	28.1% (16/57)	22.2% (16/72)
Aorta at renal arteries/in renal arteries	13.3% (2/15)	43.9% (25/57)	37.5% (27/72)
Infrarenal abdominal aorta	13.3% (2/15)	49.1% (28/57)	41.7% (30/72)
Common iliac arteries (right or left)	0%	17.5% (10/57)	13.9% (10/72)
External iliac arteries (right or left)	0%	3.5% (2/57)	2.8% (2/72)
Internal iliac arteries (right or left)	0%	1.8% (1/57)	1.4% (1/72)
Femoral arteries (right or left)	0%	0%	0%
Unknown	6.7% (1/15)	10.5% (6/57)	9.7% (7/72)

LCC: left common carotid artery; SLA: left subclavian artery; SMA: superior mesenteric artery.

^a Patients may have presented with multiple secondary/reentry tears.

^b Patient 1130090 was unable to be assessed by the core laboratory due to inadequate imaging.

Procedural Information

Procedural information is summarized in Table 13. All procedures were performed under general anesthesia. Vascular access techniques employed during the procedure included femoral artery cutdown in 72.6% of patients, percutaneous access in 58.9% of patients, and use of a conduit in 2.7% of patients (multiple access methods were possible). A surgical cutdown appeared more common in patients without a Dissection Stent. Adjunctive techniques for spinal cord protection were performed in 39.7%, including primarily cerebrospinal fluid (CSF) drainage. The majority of patients had either partial or complete coverage of the left subclavian artery (LSA), often without a revascularization procedure.

Table 13. Procedural information

Item	Result n (%)
Anesthesia Method	
General	73 (100%)
Regional	0
Local	0
Access Method^a	
Percutaneous	43 (58.9%)
Cut-Down	53 (72.6%)
Conduit	2 (2.7%)
Adjunctive Techniques to Prevent Paraplegia	
CSF Drainage	26 (35.6%)
Neurologic/Cerebral Monitoring	2 (2.7%)
Induced Hypertension	1 (1.4%)
LSA Coverage	
Complete	28 (38.4%)
Partial	15 (20.5%)
None	30 (41.1%)
LSA Revascularization Procedure	
None	58 (79.4%)
Transposed	4 (5.5%)
Bypassed	11 (15.1%)

^a Multiple access methods may have been used in a patient.

The mean procedure time was 154.9 ± 91.3 minutes and the mean procedural blood loss was 242.1 ± 315.8 ml. The mean anesthesia time was 234.2 ± 96.7 minutes. Procedure times as well as procedural blood loss appeared greater on average in patients who received a Dissection Stent, which is reasonably expected given the differences between groups in terms of number of components placed, as further described below.

Devices Placed during Index Procedure

Tables 14-16 report the number and sizes of Dissection Endovascular Grafts (nontapered and tapered) and Dissection Endovascular Stents placed at the time of the index procedure. The largest (42 mm) and smallest (22 mm) diameters, the longest (218 mm) and shortest (79 mm) lengths, and both tapered options (4 mm and 8 mm) were used among the patients enrolled in the study, supporting the clinical relevance of the available sizes. All available Dissection Stent diameters and lengths were used.

Table 14. Number and sizes (diameters and lengths) of nontapered Dissection Endovascular Graft components implanted during index procedure

Diameter (mm)	Length (mm)	N
22	79	1
	117	0
24	79	0
	117	0
26	79	1
	136	2
28	82	1
	142	4
	202	1
30	82	1
	142	6
	202	2
32	82	2
	142	9
	202	5
34	79	2
	154	3
	204	7
36	79	1
	154	9
	204	3
38	79	0
	154	2
	204	3
40	83	0
	164	0
	218	1
42	83	1
	164	0
	218	1

Table 15. Number and sizes (diameters and lengths) of tapered Dissection Endovascular Graft components implanted during index procedure

Proximal Diameter (mm)	Distal Diameter (mm)	Length (mm)	N
32	28	162	0
		202	0
	24	158	0
		196	0
34	30	159	3
		199	5
	26	156	1
		194	0
36	32	159	2
		199	6
	28	159	1
		199	1
38	34	154	0
		204	1
	30	159	1
		199	0
40	36	160	1
		210	3
	32	165	1
		205	1
42	38	160	1
		210	1
	34	160	3
		210	2

Table 16. Number and sizes (diameters and lengths) of Dissection Stent components implanted during index procedure

Diameter (mm)	Length (mm)	N
36	80	13
	120	18
	180	27
46	80	3
	120	4
	185	13

Table 17 further describes the different main body component combinations used during the initial implant procedure, as selected at the discretion of the treating physician, for patients who did not receive a Dissection Stent and for patients who received a Dissection Stent. All patients received at least one stent-graft, with nearly 80% of patients also receiving at least one Dissection Stent. Two or more Dissection Endovascular Grafts were used in approximately one-third of patients. There appeared to be differences between groups in terms of the number of components placed, where three or more components were placed in half of the patients with a Dissection Stent, whereas none of the patients in the group without a Dissection Stent received more than two components (and 40% received one component).

Table 17. Combination of components placed during the initial implant procedure

Main Body Combination	Percent Patients (number/total number)	
	Without Dissection Stent	With Dissection Stent
One Dissection Endovascular Graft (only)	40.0% (6/15)	NA
Two Dissection Endovascular Grafts (only)	60.0% (9/15)	NA
One Dissection Endovascular Graft and one Dissection Stent	NA	44.8% (26/58)
One Dissection Endovascular Graft and two Dissection Stents	NA	22.4% (13/58)
One Dissection Endovascular Graft and three Dissection Stents	NA	1.7% (1/58)
One Dissection Endovascular Graft and four Dissection Stents	NA	1.7% (1/58)
Two Dissection Endovascular Grafts and one Dissection Stent	NA	24.1% (14/58)
Two Dissection Endovascular Grafts and two Dissection Stents	NA	0%
Two Dissection Endovascular Grafts and three Dissection Stents	NA	1.7% (1/58)
Three Dissection Endovascular Grafts and one Dissection Stent	NA	3.4% (2/58)

Table 18 provides information pertaining to the location of dissection (proximal extent, primary tear, distal extent) as well as the location in which the Dissection Endovascular Graft and Dissection Stent were placed as assessed by the core laboratory according to the zone classification by Fillinger, et al.¹ Zones 2 through 4 were the most common locations for Dissection Endovascular Graft placement, while Zones 4 through 9 were the most common locations for Dissection Stent placement. Although the core laboratory noted graft placement extending into Zone 1 in 49.3%, none of the patients had coverage

of the LCC, indicating only a portion of the graft (such as along the inner curvature) extended into Zone 1.

Table 18. Dissection Stent and Dissection Endovascular Graft coverage relative to extent of dissection and primary tear location according to zone classification based on core laboratory assessment

Zone ^a		Dissection Location (pre-procedure) ^b			Device Location (at first follow-up) ^b	
		Proximal Extent	Primary Tear	Distal Extent	Dissection Endovascular Graft	Dissection Stent
Mid-point of descending thoracic aorta (approx. T6)	0	4.2% (3/72)	-	-	-	-
	1	6.9% (5/72)	-	-	49.3% (34/69)	-
	2	38.9% (28/72)	2.8% (2/72)	-	82.6% (57/69)	-
	3	37.5% (27/72)	4.2% (3/72)	-	88.4% (61/69)	-
	4	5.6% (4/72)	70.8% (51/72)	1.4% (1/72)	94.2% (65/69)	61.8% (34/55)
	5	5.6% (4/72)	15.3% (11/72)	8.3% (6/72)	68.1% (47/69)	94.5% (52/55)
	6	-	-	2.8% (2/72)	5.8% (4/69)	65.5% (36/55)
	7	-	-	2.8% (2/72)	-	65.5% (36/55)
	8	-	-	9.7% (7/72)	1.4% (1/69)	60.0% (33/55)
	9	-	-	23.6% (17/72)	1.4% (1/69)	54.5% (30/55)
	10	-	-	19.4% (14/72)	-	1.8% (1/55)
	11	-	-	19.4% (14/72)	-	1.8% (1/55)
Unk		1.4% (1/72)	6.8% (5/72)	11.1% (8/72)	1.4% (1/69)	-

Unk = unknown

^a Data are reported as zones 0-11 according to the diagram in Fillinger, et al.¹

^b Dashes indicate a value of 0%

Tables 19 and 20 report additional procedures performed (including accessory device usage) during the time of the index procedure among patients with a Dissection Stent and patients without a Dissection Stent, respectively. The majority of patients with procedures before device placement underwent carotid-subclavian bypass. Transposition

of the LSA, iliac artery angioplasty/stent placement, and other procedure types were also reported. Procedures after device deployment included transposition of the LSA, celiac artery stent placement, iliac artery angioplasty/stent placement, SMA fenestration, and other procedure types, which often involved renal artery and/or SMA stent placement. Rates of additional procedures were generally comparable between the two patient populations. However, additional procedures involving the celiac artery, SMA, and/or renal arteries (i.e., fenestration, angioplasty, stent placement) appeared to be more common in patients who received a Dissection Stent, which is consistent with these patients more often presenting initially for treatment of malperfusion as compared to patients who did not receive a Dissection Stent, who often presented for treatment of rupture.

Table 19. Additional procedures performed and accessory device usage during the index procedure in patients with a Dissection Stent

Procedure	Percent Patients (number/total number)	
	Before Device Deployment	After Device Deployment
Carotid-subclavian bypass	15.5% (9/58)	0% (0/58)
LSA transposition	5.2% (3/58)	1.7% (1/58)
Celiac artery stent	0% (0/58)	1.7% (1/58)
Iliac artery angioplasty	1.7% (1/58)	1.7% (1/58)
Iliac artery stent or stent-graft	1.7% (1/58)	8.6% (5/58)
SMA fenestration	0% (0/58)	1.7% (1/58)
Other	6.9% (4/58) ^a	22.4% (13/58) ^b

LCC: left common carotid artery; LSA: left subclavian artery; SMA: superior mesenteric artery.

^a Carotid-to-axillary bypass (n=1); transesophageal echo (n=1); exploratory laparotomy (n=1); Amplatzer plug placement to embolize the LSA (n=1).

^b SMA stent placement (n=1); esophagogastroduodenoscopy and esophagectomy (n=1); renal artery stent placement (n=2); renal artery stent placement, common iliac artery thrombectomy, and femoral patch angioplasty (n=1); renal artery stent placement, SMA stent placement, and iliofemoral bypass (n=1); dialysis catheter insertion (n=1); common iliac artery endarterectomy and patching (n=1); chest tube placement (n=1); transesophageal echo (n=2); fasciotomy (n=1); renal artery stent placement and femoral artery endarterectomy (n=1).

Table 20. Additional procedures performed and accessory device usage during the index procedure in patients without a Dissection Stent

Procedure	Percent Patients (number/total number)	
	Before Device Deployment	After Device Deployment
Carotid-subclavian bypass	6.7% (1/15)	0% (0/15)
SMA fenestration	0% (0/15)	6.7% (1/15)
Vessel closure device	0% (0/15)	13.3% (2/15)
Other	0% (0/15)	13.3% (2/15) ^a

LCC: left common carotid artery; LSA: left subclavian artery; SMA: superior mesenteric artery.

^a Femoral-femoral bypass (n=1); ballooning of true lumen of aorta in abdominal region (n=1).

The clinical utility results are presented in Table 21. The measures appeared to be comparable or generally higher in patients who received a Dissection Stent.

Table 21. Clinical utility measures

Variable	Mean ± SD (N, range)		
	Without Dissection Stent	With Dissection Stent	Total
Days in ICU	3.2 ± 2.3 (14, 1 - 10)	7.0 ± 7.3 (57, 0 - 30)	6.3 ± 6.7 (71, 0 - 30)
Days to discharge	12.5 ± 11.0 (15, 2 - 32)	11.6 ± 9.8 (58, 1 - 47)	11.8 ± 10.0 (73, 1 - 47)
Days to first bowel movement	4.1 ± 3.2 (15, 0 - 12)	4.7 ± 2.9 (48, 0 - 12)	4.6 ± 2.9 (63, 0 - 12)
Days to resumption of oral fluid intake	1.1 ± 1.0 (15, 0 - 3)	3.3 ± 6.1 (50, 0 - 35)	2.8 ± 5.5 (65, 0 - 35)
Days to resumption of regular diet	3.7 ± 4.1 (15, 0 - 16)	5.5 ± 7.3 (47, 0 - 35)	5.0 ± 6.7 (62, 0 - 35)
Mechanical ventilation (days)	0.5 ± 0.6 (15, 0 - 2)	2.0 ± 4.8 (58, 0 - 28)	1.7 ± 4.3 (73, 0 - 28)
Procedural intubation (hours)	7.7 ± 8.5 (15, 1.5 - 28)	25.8 ± 64.3 (56, 0 - 375)	22.0 ± 57.6 (71, 0 - 375)
Number of blood transfusions	1 (1, NA)	1 ± 0 (11, 1 - 1)	1 ± 0 (12, 1 - 1)

D. Safety and Effectiveness Results (Through 12 Months)

As explained above, the core laboratory-identified patients with dissection of the aorta proximal to the left subclavian artery, a length < 20 mm between the LCC and proximal extent of dissection, or with fixation site diameters >38 mm were not excluded from the hypotheses-driven and secondary endpoints analyses, because enrollment in the study was determined by site evaluation. In addition, inclusion of these patients would not favorably bias the study results.

The primary analysis of safety and effectiveness was based on the 67 evaluable patients at the 30-day time point, excluding the 6 patients without confirmed absence of bowel necrosis at the time of enrollment.

Table 22 presents the results of hypothesis testing for the primary endpoint for the Zenith Dissection Endovascular System. The 30-day survival rate was 95.5%, which met the performance goal of 79.4% ($p < 0.001$).

Table 22. Results from primary effectiveness hypothesis testing (30-day survival)

Performance Goal	30-day Survival Rate	95% Confidence Interval	P-value	Performance Goal Met
79.4%	95.5% (64/67)	87%, 99% ^a	< 0.001	Yes

^a 95% confidence interval was computed using the Exact method.

There were three patients who died within 30 days, the details of which are provided in Table 23. Each death within 30 days occurred in a patient who received a Dissection Stent.

Table 23. Patient deaths within 30 days

Patient Number	Days Post-procedure	Cause of Death	CEC Adjudication
1130012*	21	Aortic rupture	Unable to be adjudicated
1130036*	1	Aortic dissection with resultant respiratory failure, cardiac arrest	Not related: related to presenting aortic dissection
1130060	5	Brain dead due to stroke	Procedure-related

* Patient had a length < 20 mm from LCC to proximal extent of dissection, a dissection that extended proximal to the LSA, and a total aortic diameter >38 mm at level of LCC/LSA at pre-procedure based on core laboratory analysis.

Two of the six patients excluded from assessment of the primary effectiveness hypothesis also died within 30 days.

1. Additional Safety Results

Protocol Defined MAEs

The additional hypothesis-driven analysis of safety (30-day freedom from MAEs) was based on the results from 67 patients. Data from 73 patients are presented for all other safety endpoints.

The 30-day freedom from MAE rate was 71.6%, which met the performance goal of 51.2% ($p < 0.001$).

The key safety outcomes for this study are presented below in Tables 24 and 25. Adverse effects are reported in Table 27.

Table 24. Results from primary safety hypothesis testing (30-day freedom from MAEs)

Performance Goal	30-day Freedom from MAE Rate	95% Confidence Interval	P-value	Performance Goal Met
51.2%	71.6% (48/67)	59%, 82% ^a	< 0.001	Yes

^a 95% confidence interval was computed using the Exact method.

There were 19 patients who experienced MAEs within 30 days (17 patients who received a Dissection Stent and 2 patients without a Dissection Stent), as summarized below in Table 25. None of the six patients excluded from assessment of the primary safety hypothesis had a MAE within 30 days.

Table 25. Patients experiencing MAEs within 30 days

Major Adverse Event	Patients without Dissection Stent	Patients with Dissection Stent	Total	SVS Acute Patients
Bowel ischemia	0%	0%	0%	3.5% (3/85)
MI	0%	1.9% (1/52) ^a	1.5% (1/67)	1.2% (1/85)
Paraparesis/Paraplegia	6.7% (1/15)	5.8% (3/52)	6.0% (4/67)	9.4% (8/85)
Prolonged (> 72 hours) ventilatory support	0%	19.2% (10/52) ^b	14.9% (10/67)	2.4% (2/85)
Renal failure requiring dialysis	6.7% (1/15)	7.7% (4/52) ^c	7.5% (5/67)	9.4% (8/85)
Stroke	0%	9.6% (5/52) ^d	7.5% (5/67)	9.4% (8/85)

MI: myocardial infarction.

^a Patient had a length < 20 mm from LCC to proximal extent of dissection and a dissection that extended proximal to the LSA at pre-procedure based on core laboratory analysis.

^b Five patients had a length < 20 mm from LCC to proximal extent of dissection, a dissection that extended proximal to the LSA and/or a total aortic diameter > 38 mm at the level of the LCC/LSA at pre-procedure based on core laboratory analysis.

^c Four patients had a length < 20 mm from LCC to proximal extent of dissection, a dissection that extended proximal to the LSA, and/or a total aortic diameter > 38 mm at the level of the LCC/LSA at pre-procedure based on core laboratory analysis.

^d Two patients had a length < 20 mm from LCC to proximal extent of dissection and/or a dissection that extended proximal to the LSA at pre-procedure based on core laboratory analysis.

Of the MAEs that were assessed, stroke and paraplegia/paraparesis are considered the most serious. While the risk of either one occurring following endovascular repair of Type B aortic dissection is well known, further investigation into the possible circumstances was warranted.

Five patients experienced stroke within 30 days. Each stroke occurred in a patient who received a Dissection Stent and was adjudicated by the CEC to be procedure-related; no stroke was adjudicated as related to the device. The LSA was covered in three of the five patients with stroke, two of which had undergone revascularization. Two patients appear to have recovered based on normal neurological exams reported at subsequent follow-up. The other three, each without recovery, were notable for potential contributing factors such as preexisting Type A dissection, presence of calcification and thrombus in the proximal seal zone at pre-procedure, and induced hypotension during the procedure.

Four patients experienced paraplegia/paraparesis within 30 days, two recovered and two were unresolved. The two patients without resolution of symptoms had both received spinal cord protection (CSF drainage) at the time of procedure. The pre-procedure imaging for both patients was notable for spinal arteries perfused by the true and false lumens, and on follow-up imaging, both had false lumen thrombosis that extended

beyond the level of spinal cord injury, suggesting the deficits in both may have resulted from decreased perfusion of the spinal arteries secondary to false lumen thrombosis.

Not Protocol Defined MAEs

While not protocol-defined as MAEs, additional (vascular) events of interest that were reported by the sites within 30 days included rupture in 1.4% (1/52 with a Dissection Stent, 0/15 without a Dissection Stent) and retrograde dissection in 1.4% (1/52 with a Dissection Stent, 0/15 without a Dissection Stent). While there were additional reports of rupture (n=1) and retrograde dissection (n=3) between 31-365 days, each occurred in a patient with preexisting Type A dissection (i.e., none of the retrograde dissections were progression of Type B dissection to Type A dissection, as also noted in Table 27, Morbidity by category and type in all patients), underscoring the importance of an adequate proximal landing zone in non-dissected aorta.

All-Cause Mortality

With regards to the entire study population (n=73), deaths between 0-30 days, 31-180 days, and 181-365 days occurred in 6.8% (1 related, 3 unrelated, 1 unable to be adjudicated), 7.5% (1 related, 3 unrelated, 1 unable to be adjudicated by the CEC) and 6.7% (2 unrelated, 2 unable to be adjudicated by the CEC), respectively, and included patients from both groups (11 with a Dissection Stent, 3 without a Dissection Stent). Death rates between 0-30 days and 31-365 days were reported in the SVS dataset at 10.6% and 15.8%, respectively. Table 26 provides the details for all patient who died within 365 days.

Table 26. Patient deaths within 365 days

Patient Number	Days After Procedure	Cause of Death	CEC Adjudication
1130001 ^a	57	Type A aortic dissection with rupture	Not related: related to preexisting Type A dissection prior to device deployment
1130012 ^a	21	Aortic rupture	Unable to be adjudicated
1130015 ^a	1	Ischemic bowel	Not related: related to a preexisting condition
1130022 ^a	3	Multiple organ failure	Not related: related to celiac artery and SMA occlusions prior to Dissection Stent placement
1130036 ^a	1	Aortic dissection with resultant respiratory failure, cardiac arrest	Not related: related to presenting aortic dissection
1130039 ^a	220	Multiple organ failure	Not related: patient did not meet inclusion criteria

Patient Number	Days After Procedure	Cause of Death	CEC Adjudication
1130049	170	Angiosarcoma, cancer	Not related: related to other condition
1130060 ^a	5	Brain dead due to stroke	Procedure-related
1130065	66	Unknown	Procedure-related: post-operatively the patient was ventilated and had a stroke; however, the terminal event is not clear
1130067	96	Unknown, found dead at home	Unable to be adjudicated
1130084 ^a	330	Atherosclerotic cardiovascular disease	Unable to be adjudicated
1130087 ^a	306	Unknown	Unable to be adjudicated
1230007	240	Respiratory failure	Not related: related to pneumonia with preexisting lung cancer and COPD
1230009	177	Ischemic heart disease	Not related: related to preexisting condition

Note: Patient numbers that are italicized indicate those who did not have confirmed absence of bowel necrosis at the time of enrollment and were therefore excluded from hypothesis testing.

^a Patient had a length < 20 mm from LCC to proximal extent of dissection, a dissection that extended proximal to the LSA, and/or a total aortic diameter > 38 mm at the level of the LCC/LSA at pre-procedure based on core laboratory analysis.

Adverse Effects that Occurred in the PMA Clinical Study

Table 27 reports the frequency of all adverse events according to organ system category and event type in the overall patient population through 12 months. The occurrence of adverse events was not unexpected given the extent of comorbid medical conditions and disease among the total patient population as well as the prevalence of early and late events in similar categories for patients undergoing endovascular treatment for acute, complicated Type B aortic dissection, as reported in the SVS dataset.

Table 27. Morbidity by category and type in all patients

Category	Type	Percent Patients (number/total number)		
		0-30 Days	31-180 Days	181-365 Days
Access site/vessel		9.6% (7/73)	3.0% (2/67)	0% (0/60)
	Dehiscence	0% (0/73)	0% (0/67)	0% (0/60)
	Hematoma	5.5% (4/73)	0% (0/67)	0% (0/60)
	Hernia	0% (0/73)	0% (0/67)	0% (0/60)
	Infection	0% (0/73)	1.5% (1/67)	0% (0/60)
	Pseudoaneurysm	2.7% (2/73)	0% (0/67)	0% (0/60)
	Seroma	2.7% (2/73)	1.5% (1/67)	0% (0/60)
Cardiovascular		13.7% (10/73)	4.5% (3/67)	1.7% (1/60)
	Cardiac arrhythmia	6.8% (5/73)	1.5% (1/67)	1.7% (1/60)
	Cardiac ischemia	1.4% (1/73)	1.5% (1/67)	0% (0/60)
	Congestive heart failure	0% (0/73)	1.5% (1/67)	0% (0/60)
	Myocardial infarction	1.4% (1/73)	0% (0/67)	0% (0/60)
	Refractory hypertension	4.1% (3/73)	0% (0/67)	0% (0/60)

Category	Type	Percent Patients (number/total number)		
		0-30 Days	31-180 Days	181-365 Days
Cerebrovascular/neurologic		11.0% (8/73)	0% (0/67)	1.7% (1/60)
	Paraplegia	2.7% (2/73)	0% (0/67)	0% (0/60)
	Paraparesis	4.1% (3/73)	0% (0/67)	0% (0/60)
	Transient ischemic attack	0% (0/73)	0% (0/67)	0% (0/60)
	Stroke	6.8% (5/73)	0% (0/67)	1.7% (1/60)
Gastrointestinal		12.3% (9/73)	0% (0/67)	3.3% (2/60)
	Bleeding	1.4% (1/73)	0% (0/67)	0% (0/60)
	Bowel ischemia	1.4% (1/73)	0% (0/67)	3.3% (2/60)
	Infection	4.1% (3/73)	0% (0/67)	0% (0/60)
	Bowel obstruction	0% (0/73)	0% (0/67)	0% (0/60)
	Paralytic ileus > 4 days	5.5% (4/73)	0% (0/67)	0% (0/60)
Pulmonary		21.9% (16/73)	3.0% (2/67)	1.7% (1/60)
	COPD	0% (0/73)	3.0% (2/67)	1.7% (1/60)
	Hemothorax	1.4% (1/73)	0% (0/67)	0% (0/60)
	Pleural effusion	16.4% (12/73)	0% (0/67)	0% (0/60)
	Pneumonia	2.7% (2/73)	0% (0/67)	0% (0/60)
	Pneumothorax	0% (0/73)	0% (0/67)	0% (0/60)
	Pulmonary edema	1.4% (1/73)	0% (0/67)	0% (0/60)
	Pulmonary embolism	1.4% (1/73)	0% (0/67)	0% (0/60)
Renal/urologic		17.8% (13/73)	6.0% (4/67)	5.0% (3/60)
	Renal failure ^a	8.2% (6/73)	1.5% (1/67)	1.7% (1/60)
	Urinary tract infection ^b	8.2% (6/73)	4.5% (3/67)	3.3% (2/60)
	Serum creatinine rise ^c	2.7% (2/73)	0% (0/67)	1.7% (1/60)
Vascular		8.2% (6/73)	4.5% (3/67)	3.3% (2/60)
	Aortic aneurysm	1.4% (1/73)	1.5% (1/67)	1.7% (1/60)
	Aortic rupture	1.4% (1/73)	1.5% (1/67)	0% (0/60)
	Aortobronchial fistula	0% (0/73)	0% (0/67)	0% (0/60)
	Aortoesophageal fistula	0% (0/73)	0% (0/67)	0% (0/60)
	Aortoenteric fistula	0% (0/73)	0% (0/67)	0% (0/60)
	Arterial thrombosis	0% (0/73)	0% (0/67)	0% (0/60)
	Coagulopathy	0% (0/73)	0% (0/67)	0% (0/60)
	Deep vein thrombosis	2.7% (2/73)	0% (0/67)	0% (0/60)
	Distal embolization ^d	0% (0/73)	0% (0/67)	0% (0/60)
	Hematoma	0% (0/73)	0% (0/67)	0% (0/60)
	Pseudoaneurysm ^e	1.4% (1/73)	0% (0/67)	0% (0/60)
	Retrograde dissection ^f	1.4% (1/73)	3.0% (2/67)	1.7% (1/60)
	Miscellaneous/other ^g	68.5% (50/73)	31.3% (21/67)	33.3% (20/60)

^a With or without dialysis.

^b Requiring antibiotic treatment.

^c > 30% above baseline resulting in a persistent value > 2.0 mg/dL.

^d With tissue loss.

^e Requiring intervention.

^f Includes retrograde progression of pre-existing Type A dissection in 3 and new Type A dissection in 1; none were considered retrograde progression of Type B dissection to Type A dissection.

^g Miscellaneous morbidity category comprises the following prespecified events: hypersensitivity/allergic reaction, multi-organ failure, sepsis, and other.

2. Additional Effectiveness Results

Additional effectiveness outcomes are presented in Tables 28 to 62, as follows.

Aortic Diameters (Total Aortic, True Lumen, False Lumen) at Follow-up

The maximum aortic diameters just distal to the celiac artery, just distal to the SMA, just distal to the right renal artery, just distal to the left renal artery, within the Dissection Endovascular Graft, and distal to the treated segment (i.e., most distal stent-graft or Dissection Stent, and within dissected aorta) were measured by the core laboratory at each time point for all patients. Compared to pre-procedure, the true lumen diameters trended larger throughout the visceral aortic segment at post-procedure. From post-procedure through 12 months, there appeared an increase (> 5 mm) in mean true lumen diameter and a decrease (> 5 mm) in mean false lumen diameter within the stent-graft. Distal to the treated segment, there appeared to be an increase (> 5 mm) in the mean total aortic diameter, with no change (≤ 5 mm) in the true and false lumen diameters.

Diameters measured at the specified locations by the core laboratory at each time point for the patients without a Dissection Stent and patients with a Dissection Stent, respectively. Compared to pre-procedure, the true lumen diameter trended smaller at the level of the SMA and both renal arteries at post-procedure in the patients without a Dissection Stent, whereas the true lumen diameter trended larger throughout the visceral aortic segment at post-procedure in the patients with a Dissection Stent. In the stent-graft region, there was an increase (> 5 mm) in average true lumen diameter, with no change (≤ 5 mm) in the average false lumen or transaortic diameters for the patients without a Dissections Stent, compared to an increase (> 5 mm) in average true lumen diameter and a decrease (> 5 mm) in the average false lumen diameter, with no change (≤ 5 mm) in total aortic diameter for patients with a Dissection Stent. In the Dissection Stent region, there was no change (≤ 5 mm) in the average total aortic, true lumen, or false lumen diameters from post-procedure to 12 months. Distal to the treated segment, there appeared an increase (> 5 mm) in the total and false lumen diameters with no change (≤ 5 mm) in true lumen diameter for patients without a Dissection Stent, compared to no change (≤ 5 mm) in the total, true, and false lumen diameters from post-procedure through 12 months for patients with a Dissection Stent. Given these data, it appears that the Dissection Graft results in favorable remodeling within the region adjacent to the Dissection Endovascular Graft, with the Dissection Stent additionally providing for further stabilization of aortic diameters distal to the stent-graft.

Change in Transaortic Diameter

Tables 28, 29, and 30 report the percentage of patients with a greater than 5 mm increase, a greater than 5 mm decrease, or no change (≤ 5 mm) in largest size in the transaortic diameter within the stent-graft region (depicted in Figure 2) for patients who did not receive a Dissection Stent, patients who received a Dissection Stent, and the total patient population, respectively, at each time point analyzed. Transaortic diameter growth (> 5 mm) in the stent-graft region was observed in 14.9% at 12 months (6/37 with a Dissection Stent, 1/10 without a Dissection Stent), including two with a net increase (> 5 mm) in false lumen diameter (both in the setting of Proximal Type I entry flow), whereas the remaining five patients had either no change (≤ 5 mm) or a net decrease (> 5 mm) in false lumen diameter.

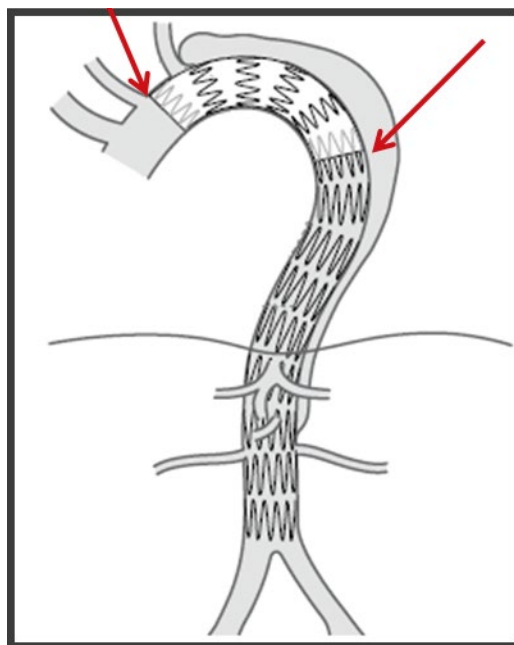


Figure 2. Diagram of the Zenith Dissection Endovascular System depicting stent-graft region (between the red arrows)

Table 28. Change in transaortic diameter within the stent-graft for patients who did not receive a Dissection Stent based on results from core laboratory analysis

Status	Percent Patients (number/total number)	
	6-month	12-month
Increase	25.0% (3/12) ^{a,b,c}	10.0% (1/10) ^a
Decrease	16.7% (2/12)	20.0% (2/10)
No change	58.3% (7/12)	70.0% (7/10)

Note: Footnotes provide the changes in true and false lumen diameters as of 12-month follow-up.

^a Patient 1130081: True lumen: -2.7 mm, False Lumen: +12.8 mm. Patient has a Type I proximal entry-flow, secondary tear in the descending thoracic aorta, and collateral flow from intercostal and paraspinal arteries. Patient had a length < 20 mm from LCC to proximal extent of dissection and a dissection that extended proximal to the LSA at pre-procedure based on core laboratory analysis.

^b Patient 1230007: True lumen: +7.8 mm, False Lumen: -2.0 mm.

^c Patient 1230010: True lumen: +12.0 mm, False Lumen: -8.4 mm.

Table 29. Change in transaortic diameter within the stent-graft for patients who received a Dissection Stent based on results from core laboratory analysis

Status	Percent Patients (number/total number)	
	6-month	12-month
Increase	16.3% (7/43) ^{a,b,c,d,e,f,g}	16.2% (6/37) ^{b,c,d,f,g,h}
Decrease	20.9% (9/43)	27.0% (10/37)
No change	62.8% (27/43)	56.8% (21/37)

^a Patient 1130017: True lumen: -0.6 mm, False Lumen: +8.3 mm. The true lumen has expanded and the false lumen has decreased. The thoracic false lumen is completely thrombosed.

^b Patient 1130074: True lumen: +11.6 mm, False Lumen: -3.7 mm.

^c Patient 1130006: True lumen: +5.7 mm, False Lumen: -0.5 mm.

^d Patient 1130044: True lumen: -1.2 mm, False Lumen: +7.6 mm. Patient has a Type I proximal entry-flow. Patient had a length < 20 mm from LCC to proximal extent of dissection and a dissection that extended proximal to the LSA at pre-procedure based on core laboratory analysis.

^e Patient 1130057: True lumen: -2.6 mm, False Lumen: +6.9 mm. Patient has collateral flow from the paraspinal arteries.

^f Patient 1130037: True lumen: +19.5 mm, False Lumen: -7.0 mm.

^g Patient 1130052: True lumen: +24.3 mm, False Lumen: -17.9 mm.

^h Patient 1130050: True lumen: +1.2 mm, False Lumen: +4.5 mm. Patient has collateral flow from the spinal arteries.

Table 30. Change in transaortic diameter within the stent-graft for all patients based on results from core laboratory analysis

Status	Percent Patients (number/total number)	
	6-month	12-month
Increase	18.2% (10/55)	14.9% (7/47)
Decrease	20.0% (11/55)	25.5% (12/47)
No change	61.8% (34/55)	59.6% (28/47)

Table 31 reports the percentage of patients with a greater than 5 mm increase, a greater than 5 mm decrease, or no change (≤ 5 mm) in largest size in the transaortic diameter within the Dissection Stent region (depicted in Figure 3). Transaortic diameter growth (> 5 mm) in the Dissection Stent region was observed in 38.5% at 12 months, including six with a net increase (> 5 mm) in false lumen diameter (each in the setting of false lumen perfusion from secondary tears and patent collateral vessels), whereas the remaining nine patients had no change (≤ 5 mm) in false lumen diameter.

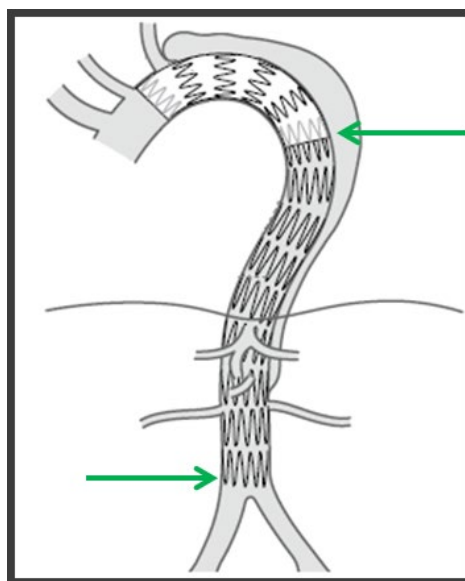


Figure 3. Diagram of Zenith Dissection Endovascular System depicting Dissection Stent region (between the green arrows)

Table 31. Change in transaortic diameter within the Dissection Stent region based on results from core laboratory analysis

Status	Percent Patients (number/total number)	
	6-month	12-month
Increase	20.5% (9/44) ^{a-i}	38.5% (15/39) ^{d-r}
Decrease	4.5% (2/44)	5.1% (2/39)
No change	75.0% (33/44)	56.4% (22/39)

Note: Footnotes provide the changes in true and false lumen diameters as of 12-month follow-up.

^a Patient 1130020: True lumen: +3.6 mm, False Lumen: -3.8 mm.

^b Patient 1130007: True lumen: +2.6 mm, False Lumen: +0.9 mm. At 6 months, growth was potentially due to a secondary tear in the descending thoracic aorta. At 12 months, the true lumen had expanded and the thoracic false lumen was completely thrombosed.

^c Patient 1130017: True lumen: -0.6 mm, False Lumen: +10.5 mm. Patient has a secondary tear at the right renal artery and collateral flow from the lumbar arteries.

^d Patient 1130035: True lumen: +2.4 mm, False Lumen: +5.0 mm. Patient has a completely thrombosed thoracic false lumen, but a secondary tear at the right renal artery and collateral flow from the paraspinal and lumbar arteries.

^e Patient 1130038: True lumen: +4.0 mm, False Lumen: +4.5 mm. Patient has a completely thrombosed thoracic false lumen, but a secondary tear at the infrarenal aorta and collateral flow from the lumbar arteries.

^f Patient 1130085: True lumen: -1.9 mm, False Lumen: 14.3 mm. Patient has secondary tears in the descending thoracic and infrarenal aorta and collateral flow from the paraspinal and lumbar arteries.

^g Patient 1130074: True lumen: +6.0 mm, False Lumen: +8.1 mm. Patient has a secondary tear in the infrarenal aorta and collateral flow from the paraspinal and lumbar arteries.

^h Patient 1130086: True lumen: +7.4 mm, False Lumen: +4.0 mm. Patient has secondary tears in the descending thoracic aorta and at the SMA as well as collateral flow from the paraspinal and lumbar arteries.

ⁱ Patient 1130037: True lumen: +3.8 mm, False Lumen: +2.0 mm. Patient has a completely thrombosed thoracic false lumen, but has a secondary tear at the right renal artery and collateral flow from the lumbar arteries.

^j Patient 1130006: True lumen: -1.8 mm, False Lumen: +9.2 mm. Patient has a Type I proximal entry-flow and collateral flow from the lumbar arteries. Patient had a length < 20 mm from LCC to proximal extent of

dissection, a dissection that extended proximal to the LSA, and an aortic diameter >38 mm at the level of the LCC/LSA at pre-procedure based on core laboratory analysis.

^k Patient 1130043: True lumen: +1.0 mm, False Lumen: +4.5 mm. Patient has a completely thrombosed thoracic false lumen, but has a secondary tear at the infrarenal aorta and celiac artery and collateral flow from the lumbar arteries.

^l Patient 1130064: True lumen: -0.9 mm, False Lumen: +6.0 mm. Patient has secondary tears in the descending thoracic and infrarenal aorta and collateral flow from the paraspinal and lumbar arteries.

^m Patient 1130069: True lumen: +7.6 mm, False Lumen: +2.2 mm.

ⁿ Patient 1130002: True lumen: +1.0 mm, False Lumen: +4.9 mm. Patient has a completely thrombosed thoracic false lumen, but has secondary tears at the celiac artery and SMA and collateral flow from the lumbar arteries.

^o Patient 1130057: True lumen: +2.8 mm, False Lumen: +4.4 mm. Patient has a partially thrombosed abdominal false lumen, but has collateral flow from the paraspinal artery.

^p Patient 1130023: True lumen: -1.6 mm, False Lumen: +10.2 mm. Patient has an unknown entry-flow, a secondary tear at the SMA, and collateral flow from the paraspinal and lumbar arteries.

^q Patient 1130070: True lumen: -3.5 mm, False Lumen: +8.8 mm. Patient has a secondary tear at the left renal artery and collateral flow from the paraspinal and lumbar arteries.

^r Patient 1130058: True lumen: +2.2 mm, False Lumen: +3.0 mm. Patient has a completely thrombosed thoracic false lumen, but has secondary tears at the right renal and celiac arteries and collateral flow from the lumbar arteries.

Tables 32, 33, and 34 report the percentage of patients with a greater than 5 mm increase, a greater than 5 mm decrease, or no change (≤ 5 mm) in largest size in the transaortic diameter distal to the treated segment for patients who did not receive a Dissection Stent, patients who received a Dissection Stent, and the total patient population, respectively, at each time point analyzed. As with the other tables reporting a change in size, the denominators reflect the number of patients with a baseline exam who also had adequate imaging extending to the level of interest, which in this case was beyond the level of the treated segment. Transaortic diameter growth (> 5 mm) distal to the treated segment was observed in 40.7% at 12 months (8 with a Dissection Stent, 3 without a Dissection Stent), including seven with a net increase (> 5 mm) in false lumen diameter (each in the setting of false lumen perfusion from secondary tears and patent collateral vessels), one with a net decrease (> 5 mm) in false lumen diameter, and three with no change (≤ 5 mm) in false lumen diameter.

Table 32. Change in transaortic diameter distal to the treated segment and within dissected aorta for patients who did not receive a Dissection Stent based on results from core laboratory analysis

Status	Percent Patients (number/total number)	
	6-month	12-month
Increase	16.7% (1/6) ^a	60.0% (3/5) ^{a-c}
Decrease	0%	0%
No change	83.3% (5/6)	40.0% (2/5)

Note: Footnotes provide the changes in true and false lumen diameters as of 12-month follow-up.

^a Patient 1230010: True lumen: +1.1 mm, False Lumen: +5.7 mm. Patient has secondary tears at the infrarenal aorta and at the celiac artery and collateral flow from the intercostal, paraspinal, and lumbar arteries.

^b Patient 1130027: True lumen: -0.6 mm, False Lumen: +6.4 mm. Patient has collateral flow from the intercostal arteries.

^c Patient 1130081: True lumen: -3.0 mm, False Lumen: +9.7 mm. Patient has a Type I proximal entry-flow, a secondary tear in the descending thoracic aorta, and collateral flow from the intercostal and paraspinal arteries. Patient had a length < 20 mm from LCC to proximal extent of dissection and a dissection that extended proximal to the LSA at pre-procedure based on core laboratory analysis.

Table 33. Change in transaortic diameter distal to the treated segment and within dissected aorta for patients who received a Dissection Stent based on results from core laboratory analysis

Status	Percent Patients (number/total number)	
	6-month	12-month
Increase	13.0% (3/23) ^{a-c}	36.4% (8/22) ^{a-h}
Decrease	0%	0%
No change	87.0% (20/23)	63.6% (14/22)

Note: Footnotes provide the changes in true and false lumen diameters as of 12-month follow-up.

^a Patient 1130076: True lumen: +7.3 mm, False Lumen: +1.9 mm. Patient has a partially thrombosed thoracic false lumen, but has a secondary tear at the left renal artery and collateral flow from the lumbar arteries.

^b Patient 1130037: True lumen: +9.3 mm, False Lumen: +10.8 mm. Patient has a completely thrombosed thoracic false lumen, but has a secondary tear at the right renal artery and collateral flow from the lumbar arteries.

^c Patient 1130052: True lumen: +0.4 mm, False Lumen: +5.0 mm. Patient has secondary tears in the infrarenal aorta and at the celiac artery and collateral flow from the lumbar arteries.

^d Patient 1130058: True lumen: +0.3 mm, False Lumen: +5.1 mm. Patient has secondary tear at the right renal and celiac arteries and collateral flow from the lumbar arteries.

^e Patient 1130038: True lumen: +3.7 mm, False Lumen: +1.8 mm. Patient has a completely thrombosed thoracic false lumen, but has a secondary tear in the infrarenal aorta and collateral flow from the lumbar arteries.

^f Patient 1130085: True lumen: +0.9 mm, False Lumen: +13.2 mm. Patient has secondary tears in the descending thoracic and infrarenal aorta and collateral flow from the paraspinal and collateral arteries.

^g Patient 1130043: True lumen: -2.4 mm, False Lumen: +11.1 mm. Patient has a completely thrombosed thoracic false lumen, but has secondary tears in the infrarenal aorta and at the celiac artery and collateral flow from the lumbar arteries.

^h Patient 1130089: True lumen: +13.0 mm, False Lumen: -7.5 mm.

Table 34. Change in transaortic diameter distal to the treated segment and within dissected aorta for all patients based on results from core laboratory analysis

Status	Percent Patients (number/total number)	
	6-month	12-month
Increase	13.8% (4/29)	40.7% (11/27)
Decrease	0%	0%
No change	86.2% (25/29)	59.3% (16/27)

False Lumen Perfusion

Tables 35, 36, and 37 detail the sources of flow in the thoracic false lumen in patients who did not receive a Dissection Stent, patients who received a Dissection Stent, and the total patient population, respectively. It should be noted that per the definitions in the study protocol, Types I through IV are intended to describe the source(s) for flow into the false lumen via the primary entry tear, and therefore speaks to the effectiveness of the endovascular graft component in sealing the primary entry tear (analogous to the endoleak types for aneurysm repair – i.e., Type I = proximal and/or distal seal; Type II =

vessels covered by graft; Type III = graft defect/hole or overlap; Type IV = graft porosity). However, recognizing the primary entry tear is not the only source for false lumen perfusion, it was necessary to further describe sources for false lumen flow not specifically associated with the effectiveness of the stent-graft to seal the primary entry tear. Therefore, the core laboratory also noted any incidences of flow directly into the false lumen via secondary tears or collateral vessels. The majority of reports of false lumen flow during follow-up were through secondary tears or collateral vessels, the coverage/occlusion of which were at physician discretion. Seven cases of Type I proximal entry flow into the thoracic false lumen were observed through 12 months. However, each patient had evidence of an inadequate proximal landing zone (i.e., aortic diameter > 38 mm and/or length of non-dissected aorta < 20 mm) and often times also graft undersizing. Overall, the proximal Type I entry-flow rate was 6.4% at 12 months (2 with a Dissection Stent, 1 without a Dissection Stent).

Table 35. Entry-flow in the thoracic aorta for patients who did not receive a Dissection Stent based on results from core laboratory analysis

Source	Percent Patients (number/total number)			
	Post-procedure	1-month	6-month	12-month
Multiple	14.3% (1/7)	25.0% (3/12)	10.0% (1/10)	11.1% (1/9)
Type I proximal	0%	8.3% (1/12) ^a	10.0% (1/10) ^b	11.1% (1/9) ^b
Type I distal	0%	0%	0%	0%
Type II	0%	0%	0%	0%
Type III	0%	0%	0%	0%
Type IV	0%	0%	0%	0%
Type unknown	0%	0%	0%	0%
Collateral	57.1% (4/7)	41.7% (5/12)	40.0% (4/10)	44.4% (4/9)
Secondary tear	14.3% (1/7)	33.3% (4/12)	10.0% (1/10)	11.1% (1/9)
Total patients	57.1% (4/7)	50.0% (6/12)	50.0% (5/10)	44.4% (4/9)

^a Patient 1130079 had a Type I proximal entry-flow noted at 1 month in the likely setting of graft undersizing as well as an inadequate proximal landing zone (diameter and length) relative to the location of graft placement according to measurements by the core laboratory. The patient was treated with ancillary devices to mitigate the entry-flow. The patient also presented with preexisting Type A dissection according to CEC adjudication.

^b Patient 1130081 had a Type I proximal entry-flow first noted at 54 days post-procedure (unscheduled visit) in the likely setting of an inadequate proximal landing zone (length) relative to the location of graft placement according to measurements by the core laboratory. This entry-flow has persisted through 12 months. No secondary interventions have been performed at this time to treat this entry-flow.

Table 36. Entry-flow in the thoracic aorta for patients who received a Dissection Stent based on results from core laboratory analysis

Source	Percent Patients (number/total number)			
	Post-procedure	1-month	6-month	12-month
Multiple	35.7% (10/28)	16.2% (6/37)	26.8% (11/41)	15.8% (6/38)
Type I proximal	3.6% (1/28) ^a	8.1% (3/37) ^{b-d}	4.9% (2/41) ^{a,c}	5.3% (2/38) ^{c,e}
Type I distal	0%	0%	0%	0%

Source	Percent Patients (number/total number)			
	Post-procedure	1-month	6-month	12-month
Type II	0%	0%	0%	0%
Type III	0%	0%	0%	0%
Type IV	0%	0%	0%	0%
Type unknown	0%	2.7% (1/37)	2.4% (1/41)	2.6% (1/38)
Collateral	57.1% (16/28)	43.2% (16/37)	41.5% (17/41)	36.8% (14/38)
Secondary tear	39.3% (11/28)	27.0% (10/37)	34.1% (14/41)	18.4% (7/38)
Total patients	64.3% (18/28)	62.2% (23/37)	51.2% (21/41)	47.4% (18/38)

^a Patient 1130087 had a Type I proximal entry-flow noted at post-procedure and at 6 months in the likely setting of an inadequate proximal landing zone (length) relative to the location of graft placement according to measurements by the core laboratory. The patient died 306 days post-procedure (CEC unable to adjudicate) with no secondary interventions performed to treat this entry-flow.

^b Patient 1130025 had a Type I proximal entry-flow noted at 1 month in the likely setting of graft undersizing as well as an inadequate proximal landing zone (diameter and length) relative to the location of graft placement according to measurements by the core laboratory. The entry-flow was completely resolved at 6 months.

^c Patient 1130006 had a Type I proximal entry-flow that was treated with surgical repair in the likely setting of graft undersizing as well as an inadequate proximal landing zone (diameter and length) relative to the location of graft placement according to measurements by the core laboratory. The patient underwent a surgical repair involving the ascending aorta and arch 153 days post-procedure. The Type I proximal entry-flow has persisted through 2 years.

^d Patient 1130082 had a Type I proximal entry-flow noted at 1 month in the likely setting of graft undersizing as well as an inadequate proximal landing zone (length) relative to the location of graft placement according to measurements by the core laboratory. No secondary interventions have been performed at this time to treat this entry-flow.

^e Patient 1130044 had a Type I proximal entry-flow noted at 12 months in the likely setting of graft undersizing as well as an inadequate proximal landing zone (length) relative to the location of graft placement according to measurements by the core laboratory. The Type I proximal entry-flow has persisted through 2 years. No secondary interventions have been performed at this time to treat this entry-flow.

Table 37. Entry-flow in the thoracic aorta for all patients based on results from core laboratory analysis

Source	Percent Patients (number/total number)			
	Post-procedure	1-month	6-month	12-month
Multiple	31.4% (11/35)	18.4% (9/49)	23.5% (12/51)	14.9% (7/47)
Type I proximal	2.9% (1/35)	8.2% (4/49)	5.9% (3/51)	6.4% (3/47)
Type I distal	0%	0%	0%	0%
Type II	0%	0%	0%	0%
Type III	0%	0%	0%	0%
Type IV	0%	0%	0%	0%
Type unknown	0%	2.0% (1/49)	2.0% (1/51)	2.1% (1/47)
Collateral	57.1% (20/35)	42.9% (21/49)	41.2% (21/51)	38.3% (18/47)
Secondary tear	34.3% (12/35)	28.6% (14/49)	29.4% (15/51)	17.0% (8/47)
Total patients	62.9% (22/35)	59.2% (29/49)	51.0% (26/51)	46.8% (22/47)

Tables 38, 39, and 40 detail the sources of entry-flow in the abdominal false lumen in patients who did not receive a Dissection Stent, patients who received a Dissection Stent, and the total patient population, respectively. The majority of patients had abdominal

false lumen flow through secondary tears and/or collateral vessels, the coverage/occlusion of which were at physician discretion. The single patient with Type I proximal entry-flow in the abdominal aorta is one of the same patients who was noted to have thoracic false lumen perfusion through proximal Type I entry-flow in the setting of apparent graft undersizing as well as an inadequate proximal landing zone (diameter and length) based on core laboratory measurements relative to the location of graft placement.

Table 38. Entry-flow in the abdominal aorta for patients who did not receive a Dissection Stent based on results from core laboratory analysis

Source	Percent Patients (number/total number)			
	Post-procedure	1-month	6-month	12-month
Multiple	28.6% (2/7)	20.0% (2/10)	22.2% (2/9)	33.3% (2/6)
Type I proximal	0%	0%	0%	0%
Type I distal	0%	0%	0%	0%
Type II	0%	0%	0%	0%
Type III	0%	0%	0%	0%
Type IV	0%	0%	0%	0%
Type unknown	0%	0%	0%	0%
Collateral	42.9% (3/7)	40.0% (4/10)	44.4% (4/9)	33.3% (2/6)
Secondary tear	28.6% (2/7)	20.0% (2/10)	33.3% (3/9)	50.0% (3/6)
Total patients	42.9% (3/7)	40.0% (4/10)	55.6% (5/9)	50.0% (3/6)

Table 39. Entry-flow in the abdominal aorta for patients who received a Dissection Stent based on results from core laboratory analysis

Source	Percent Patients (number/total number)			
	Post-procedure	1-month	6-month	12-month
Multiple	82.1% (23/28)	70.3% (26/37)	63.2% (24/38)	66.7% (26/39)
Type I proximal	0%	2.7% (1/37) ^a	0%	0%
Type I distal	0%	0%	0%	0%
Type II	0%	0%	0%	0%
Type III	0%	0%	0%	0%
Type IV	0%	0%	0%	0%
Type unknown	0%	0%	2.6% (1/38)	0% (0/39)
Collateral	92.9% (26/28)	81.1% (30/37)	84.2% (32/38)	76.9% (30/39)
Secondary tear	89.3% (25/28)	75.7% (28/37)	71.1% (27/38)	74.4% (29/39)
Total patients	100% (28/28)	89.2% (33/37)	92.1% (35/38)	84.6% (33/39)

^a Patient 1130006 underwent a surgical repair 153 days post-procedure in the likely setting of graft undersizing as well as an inadequate proximal landing zone (diameter and length) relative to the location of graft placement according to measurements by the core laboratory. The patient underwent a surgical repair involving the ascending aorta and arch 153 days post-procedure.

Table 40. Entry-flow in the abdominal aorta for all patients based on results from core laboratory analysis

Source	Percent Patients (number/total number)			
	Post-procedure	1-month	6-month	12-month
Multiple	71.4% (25/35)	59.6% (28/47)	55.3% (26/47)	62.2% (28/45)
Type I proximal	0%	2.1% (1/47)	0%	0%

Source	Percent Patients (number/total number)			
	Post-procedure	1-month	6-month	12-month
Type I distal	0%	0%	0%	0%
Type II	0%	0%	0%	0%
Type III	0%	0%	0%	0%
Type IV	0%	0%	0%	0%
Type unknown	0%	0%	2.1% (1/47)	0%
Collateral	82.9% (29/35)	72.3% (34/47)	76.6% (36/47)	71.1% (32/45)
Secondary tear	77.1% (27/35)	63.8% (30/47)	63.8% (30/47)	71.1% (32/45)
Total patients	88.6% (31/35)	78.7% (37/47)	85.1% (40/47)	80.0% (36/45)

False Lumen Status

Tables 41, 42, and 43 present data for false lumen status within the stent-graft region for patients who did not receive a Dissection Stent, patients who received a Dissection Stent, and the total patient population, respectively. There were no patients with a patent false lumen in the region of the stent-graft at 12 months, and 78.3% had complete thrombosis (including those no longer with an apparent false lumen), which appeared greater in the patients with a Dissection Stent (86.5%) compared to the patients without a Dissection Stent (44.4%).

Table 41. Status of false lumen within the stent-graft for patients who did not receive a Dissection Stent based on results from core laboratory analysis

Status	Percent Patients (number/total number)			
	Post-procedure	1-month	6-month	12-month
Patent	0%	8.3% (1/12) ^a	0%	0%
Partially thrombosed	57.1% (4/7)	41.7% (5/12)	50.0% (5/10)	55.6% (5/9)
Completely thrombosed	42.9% (3/7)	50.0% (6/12)	40.0% (4/10)	33.3% (3/9)
No apparent false lumen	0% (0/7)	0% (0/12)	10.0% (1/10)	11.1% (1/9)

^a Patient 1230010: false lumen flow through a secondary tear in the descending thoracic aorta as well as collateral vessels reported at this time point; the false lumen in the stent-graft region was partially thrombosed at 6 and 12 months.

Table 42. Status of false lumen within the stent-graft for patients who received a Dissection Stent based on results from core laboratory analysis

Status	Percent Patients (number/total number)			
	Post-procedure	1-month	6-month	12-month
Patent	0%	0%	0%	0%
Partially thrombosed	46.4% (13/28)	41.7% (15/36)	29.3% (12/41)	13.5% (5/37)
Completely thrombosed	53.6% (15/28)	52.8% (19/36)	61.0% (25/41)	78.4% (29/37)
No apparent false lumen	0% (0/28)	5.6% (2/36)	9.8% (4/41)	8.1% (3/37)

Table 43. Status of false lumen within the stent-graft for all patients based on results from core laboratory analysis

Status	Percent Patients (number/total number)			
	Post-procedure	1-month	6-month	12-month
Patent	0%	2.1% (1/48)	0%	0%
Partially thrombosed	48.6% (17/35)	41.7% (20/48)	33.3% (17/51)	21.7% (10/46)
Completely thrombosed	51.4% (18/35)	52.1% (25/48)	56.9% (29/51)	69.6% (32/46)
No apparent false lumen	0% (0/35)	4.2% (2/48)	9.8% (5/51)	8.7% (4/46)

Table 44 presents data for false lumen status within the Dissection Stent region over time based on core laboratory analysis. The rate of false lumen patency decreased over time whereby the majority of patients (97.5%) had either partial thrombosis, complete thrombosis, or no apparent false lumen any longer within the Dissection Stent region at 12 months. The one patient (2.6%) with a patent false lumen at 12 months (also with false lumen perfusion from secondary tears and patent collaterals) had a partially thrombosed false lumen in this region at subsequent follow-up.

Table 44. Status of false lumen within the Dissection Stent based on results from core laboratory analysis

Status	Percent Patients (number/total number)			
	Post-procedure	1-month	6-month	12-month
Patent	10.7% (3/28) ^{a,b,c}	11.1% (4/36) ^{c,d,e,f}	2.4% (1/41) ^g	2.6% (1/39) ^h
Partially thrombosed	85.7% (24/28)	83.3% (30/36)	80.5% (33/41)	79.5% (31/39)
Completely thrombosed	3.6% (1/28)	5.6% (2/36)	14.6% (6/41)	15.4% (6/39)
No apparent false lumen	0%	0%	2.4% (1/41) ⁱ	2.6% (1/39) ⁱ

^a Patient 1130074: the false lumen in the Dissection Stent region was not assessed at 1 month and was partially thrombosed at 6 and 12 months.

^b Patient 1130067: the patient died 96 days post-procedure (CEC unable to adjudicate), prior to completing any additional follow-up visits.

^c Patient 1130082: the patient was lost-to-follow-up following the 1-month imaging.

^d Patient 1130038: the false lumen in the Dissection Stent region was partially thrombosed at 6 and 12 months.

^e Patient 1130084: the false lumen in the Dissection Stent region was partially thrombosed at post-procedure and 6 months; the patient died 330 days post-procedure (CEC unable to adjudicate), prior to completing the 12-month follow-up visit.

^f Patient 1130057: the false lumen in the Dissection Stent region was partially thrombosed at 6 and 12 months.

^g Patient 1130058: the false lumen in the Dissection Stent region was partially thrombosed at post procedure, 1 month, and 12 months.

^h Patient 1130069: the false lumen in the Dissection Stent region was partially thrombosed at post-procedure, 1 month, and 2 years. The false lumen in this region was not assessed at 6 months.

Tables 45, 46, and 47 present data for false lumen status distal to the treated segment for patients who did not receive a Dissection Stent, patients who received a Dissection Stent, and the total patient population, respectively. Distal to the treated segment, false lumen patency was noted in 17% of patients at 12 months (7 with a Dissection Stent, 1 without a

Dissection Stent). While the rate of false lumen patency distal to the treated segment initially appeared higher (at post-procedure) in the patients with a Dissection Stent, the rates were more comparable between groups by 12 months; a trend towards a higher percentage of patients with a patent false lumen distal to the treated segment is not unexpected for the group with a Dissection Stent as these patients tended to more often present with secondary tears, particularly in locations distal to the stent-graft (i.e., in the region of the branch vessels and abdominal aorta) as compared to patients who did not receive a Dissection Stent.

Table 45. Status of false lumen distal to the treated segment for patients who did not receive a Dissection Stent based on results from core laboratory analysis

Status	Percent Patients (number/total number)			
	Post-procedure	1-month	6-month	12-month
Patent	16.7% (1/6) ^a	16.7% (2/12) ^{b,c}	10.0% (1/10) ^a	11.1% (1/9) ^a
Partially thrombosed	33.3% (2/6)	25.0% (3/12)	40.0% (4/10)	22.2% (2/9)
Completely thrombosed	33.3% (2/6)	33.3% (4/12)	10.0% (1/10)	22.2% (2/9)
No apparent false lumen	16.7% (1/6)	25.0% (3/12)	40.0% (4/10)	44.4% (4/9)

^a Patient 1130081

^b Patient 1130079

^c Patient 1230010: partially thrombosed at subsequent time points

Table 46. Status of false lumen distal to the treated segment for patients who received a Dissection Stent based on results from core laboratory analysis

Status	Percent Patients (number/total number)			
	Post-procedure	1-month	6-month	12-month
Patent	57.1% (16/28) ^{a-p}	22.7% (9/35) ^{i-l,o-s}	25.6% (10/39) ^{e,f,i,l,o,p,r,t,u,v}	18.4% (7/38) ^{b,i,p,r,s,t,w}
Partially thrombosed	21.4% (6/28)	37.1% (13/35)	48.7% (19/39)	50.0% (19/38)
Completely thrombosed	3.6% (1/28)	0% (0/35)	5.1% (2/39)	5.3% (2/38)
No apparent false lumen	17.9% (5/28)	37.1% (13/35)	20.5% (8/39)	26.3% (10/38)

^a Patient 1130047: partially thrombosed at subsequent time points.

^b Patient 1130085.

^c Patient 1130088: partially thrombosed at subsequent time points.

^d Patient 1130066.

^e Patient 1130074: n/a at 1-month, partially thrombosed at subsequent time points.

^f Patient 1130087.

^g Patient 1130067.

^h Patient 1130043: partially thrombosed at subsequent time points.

ⁱ Patient 1130044.

^j Patient 1130064: partially thrombosed at subsequent time points.

^k Patient 1130082.

^l Patient 1130084.

^m Patient 1130060.

ⁿ Patient 1130052: n/a at 1-month, partially thrombosed at subsequent time points.

^o Patient 1130053: partially thrombosed at subsequent time points.

^p Patient 1130058: partially thrombosed at subsequent time points.

^q Patient 1130034: n/a at 6-month, partially thrombosed at 12-month.

^r Patient 1130038.

^s Patient 1130013.

^t Patient 1130024.

^u Patient 1130039.

^v Patient 1130035: partially thrombosed at subsequent time points.

^w Patient 1130068.

Table 47. Status of false lumen distal to the treated segment for all patients based on results from core laboratory analysis

Status	Percent Patients (number/total number)			
	Post-procedure	1-month	6-month	12-month
Patent	50.0% (17/34)	23.4% (11/47)	22.4% (11/49)	17.0% (8/47)
Partially thrombosed	23.3% (8/34)	34.0% (16/47)	46.9% (23/49)	44.7% (21/47)
Completely thrombosed	8.8% (3/34)	8.5% (4/47)	6.1% (3/49)	8.5% (4/47)
No apparent false lumen	17.6% (6/34)	34.0% (16/47)	24.5% (12/49)	29.8% (14/47)

Progression of Dissection

Tables 48, 49, and 50 report the results from qualitative assessment by the core laboratory for progression of dissection during follow-up for patients who did not receive a Dissection Stent, patients who received a Dissection Stent, and the total patient population, respectively. The counts in this section are based on imaging assessment by the core laboratory (refer also to the discussion of site-reported events as provided in the following sections: “Not Protocol Defined MAEs” and “Adverse Effects that Occurred in the PMA Clinical Study”). Two patients with progression of dissection proximally and two patients with progression of dissection distally were reported by the core laboratory within 12 months. Each report occurred in a patient with a Dissection Stent, though in none of the patients did the progression appear associated with placement of the Dissection Stent (or Dissection Endovascular Graft) given the details described in the footnotes below.

Table 48. Progression of dissection in patients who did not receive a Dissection Stent based on results from core laboratory analysis

Progression	Percent Patients (number/total number)			
	Post-procedure	1-month	6-month	12-month
Yes	0%	0%	0%	0%
No	100% (3/3)	100% (10/10)	100% (10/10)	100% (8/8)

Table 49. Progression of dissection in patients who received a Dissection Stent based on results from core laboratory analysis

Progression	Percent Patients (number/total number)			
	Post-procedure	1-month	6-month	12-month
Yes	6.7% (1/15) ^a	6.1% (2/33) ^{b,c}	2.9% (1/35) ^d	0%
No	93.3% (14/15)	93.9% (31/33)	97.1% (34/35)	100% (35/35)

^a Patient 1130060 had progression of dissection proximally, extending to Zone 0 (also with a new tear in this zone) as compared to Zone 2 at pre-procedure. The ascending aortic diameter (36.3 mm) appeared notably larger than the aortic arch diameter (28.8 mm) at pre-procedure, such that the potential for

underlying disease in the ascending aortic segment cannot be ruled out as a potential contributing factor to progression of dissection proximally.

^b Patient 1130088 had progression of dissection distally, extending to Zone 10 as compared to Zone 9 at pre-procedure, whereas the Dissection Stent had only extended to Zone 5. Abdominal false lumen perfusion through a secondary tear as well as collateral vessels was noted at the same follow-up time point, which cannot be ruled out as a potential contributing factor to progression of dissection distally.

^c Patient 1130002 had progression of dissection distally, but only within the celiac artery, not the aorta.

^d Patient 1130039 had progression of dissection proximally. The patient had preexisting Type A dissection prior to the index procedure (per CEC adjudication) as well as a patent false lumen proximal and distal to the treated segment at 6 months.

Table 50. Progression of dissection in all patients based on results from core laboratory analysis

Progression	Percent Patients (number/total number)			
	Post-procedure	1-month	6-month	12-month
Yes	5.6% (1/18)	4.7% (2/43)	2.2% (1/45)	0%
No	94.4% (17/18)	95.3% (41/43)	97.8% (44/45)	100% (43/43)

Branch Vessel Patency

Table 51 reports the patency status of the branch vessels (left subclavian, spinal, celiac, superior mesenteric, renal, and common iliac arteries), as assessed by the core laboratory at each time point for all patients. The only aortic branch vessel occlusions noted by the core laboratory during follow-up involved the left subclavian artery; there were no spinal, celiac, SMA, or renal artery occlusions, and the few patients with common iliac artery occlusions at follow-up also had occlusion noted at pre-procedure.

Table 51. Patency of branch vessels in all patients based on results from core laboratory analysis

Artery Status	Percent Patients (number/total number)				
	Pre-procedure	Post-procedure	1-month	6-month	12-month
LSA					
Patent	100% (71/71)	65.7% (23/35)	69.4% (34/49)	76.5% (39/51)	75.0% (36/48)
Occluded	0%	2.9% (1/35)	6.1% (3/49)	7.8% (4/51)	4.2% (2/48)
Revascularization	0%	31.4% (11/35)	24.5% (12/49)	15.7% (8/51)	18.8% (9/48)
Unknown	0%	0%	0%	0%	2.1% (1/48)
Spinal artery					
Patent	100.0% (72/72)	100% (35/35)	100% (49/49)	100% (51/51)	100% (48/48)
Occluded	0%	0%	0%	0%	0%
Unknown	0%	0%	0%	0%	0%
Celiac artery					
Patent	98.6% (69/70)	100% (34/34)	100% (48/48)	100% (51/51)	95.8% (46/48)
Occluded	1.4% (1/70)	0%	0%	0%	0%
Unknown	0%	0%	0%	0%	4.2% (2/48)
SMA					
Patent	100% (68/68)	100% (35/35)	100% (49/49)	100% (50/50)	97.9% (47/48)
Occluded	0%	0%	0%	0%	0%
Unknown	0%	0%	0%	0%	2.1% (1/48)
Left renal artery					
Patent	100% (68/68)	100% (35/35)	100% (48/48)	100% (50/50)	100% (47/47)
Occluded	0%	0%	0%	0%	0%
Unknown	0%	0%	0%	0%	0%

Artery Status	Percent Patients (number/total number)				
	Pre-procedure	Post-procedure	1-month	6-month	12-month
Right renal artery					
Patent	98.5% (66/67)	100% (35/35)	100% (49/49)	100% (50/50)	100% (46/46)
Occluded	1.5% (1/67)	0%	0%	0%	0%
Unknown	0%	0%	0%	0%	0%
Left CIA					
Patent	100% (62/62)	97.1% (33/34)	100% (48/48)	98.0% (48/49)	100% (46/46)
Occluded	0%	0%	0%	0%	0%
Unknown	0%	2.9% (1/34)	0%	2.0% (1/49)	0%
Right CIA					
Patent	93.5% (58/62)	97.1% (33/34)	97.9% (47/48)	96.0% (47/49)	95.7% (44/46)
Occluded	6.5% (4/62)	0%	2.1% (1/48)	2.0% (1/49)	4.3% (2/46)
Unknown	0%	2.9% (1/34)	0%	2.0% (1/49)	0%

Device Integrity

Tables 52, 53, and 54 report the occurrence of device integrity findings at each follow-up time point for patients who did not receive a Dissection Stent, patients who received a Dissection Stent, and the total patient population, respectively, as determined by the core laboratory. There were no device integrity losses (i.e., stent fractures) within 12 months, only isolated observations of graft kink in one patient, device compression in two patients (involving the Dissection Endovascular Graft in one and the Dissection Stent in one), and increasing overlap between adjacent z-stent segments of a Dissection Stent in one, none of which were associated with adverse clinical sequelae or the need for reintervention.

Table 52. Device integrity findings in patients who did not receive a Dissection Stent based on results from core laboratory analysis

Finding	Number of Occurrences			
	Post-procedure	1-month	6-month	12-month
Kink	0	0	0	0
Stent fracture	0	0	0	0
Device compression	0	0	0	0
Device infolding	0	0	0	0
Other	0	0	0	0

Table 53. Device integrity findings in patients who received a Dissection Stent based on results from core laboratory analysis

Finding	Number of Occurrences			
	Post-procedure	1-month	6-month	12-month
Kink	0	0	0	1 ^c
Stent fracture	0	0	0	0
Device compression	0	0	2 ^{a,d}	1 ^d
Device infolding	0	0	0	0
Other	0	0	1 ^b	0

^a Patient 1130039 had device compression of the stent-graft; patient had pre-existing Type A dissection.

^b Patient 1130017 had increasing overlap of the 5th and 6th rings of the proximal Dissection Stent; no migration or component separation noted.

^c Patient 1130069 had a kink in the stent-graft; descending thoracic aorta with notable angulation/curvature at pre-procedure.

^d Patient 1130058 had device compression of the Dissection Stent; patient had slight true lumen diameter decrease in setting of false lumen perfusion from secondary tears and collateral vessels as well as false lumen diameter increase along treated region.

Table 54. Device integrity findings in all patients based on results from core laboratory analysis

Finding	Number of Occurrences			
	Post-procedure	1-month	6-month	12-month
Kink	0	0	0	1
Stent fracture	0	0	0	0
Device compression	0	0	2	1
Device infolding	0	0	0	0
Other	0	0	1	0

Device Migration

Migration was defined as antegrade or retrograde movement of the proximal or distal component of the endoprosthesis greater than 10 mm relative to anatomical landmarks identified on the first post-operative CT scan, as identified by the core laboratory and confirmed by the CEC. Tables 55, 56, and 57 report device migration results based on core laboratory analysis and CEC confirmation for patients who did not receive a Dissection Stent, patients who received a Dissection Stent, and the total patient population, respectively. There were 4 reports of CEC-confirmed migration > 10 mm within 12 months, each of which occurred in a patient who received a Dissection Stent, though there was no migration of the Dissection Stent, only migration of the Dissection Endovascular Graft. However, in all cases, there appeared an inadequate proximal landing zone length (< 20 mm of nondissected aorta) as well as graft undersizing in three based on measurements of the core laboratory relative to the location of graft placement. None of the patients required a secondary intervention to treat migration according to the site. The rates of migration in the current study (6.0% at 6 months, 2.2% at 12 months) appear comparable to the rates observed in the acute patient cohort from the feasibility study involving the previous graft design that had barbs (6.8% at 6 months, 4.8% at 12 months).

Table 55. Device migration in patients who did not receive a Dissection Stent based on results from core laboratory analysis and CEC confirmation

Finding	Percent Patients (number/total number)	
	6-month	12-month
Migration (> 10 mm)	0% (0/9)	0% (0/8)

Table 56. Device migration in patients who received a Dissection Stent based on results from core laboratory analysis and CEC confirmation

Finding	Percent Patients (number/total number)	
	6-month	12-month
Migration (> 10 mm)	7.3% (3/41) ^{a,b,c}	2.6% (1/38) ^d

^a Patient 1130020 had caudal migration of the Dissection Endovascular Graft in the likely setting of graft undersizing as well as an inadequate proximal landing zone (length) relative to the location of graft placement according to measurements by the core laboratory. No secondary interventions have been performed to treat this migration

^b Patient 1130074 had caudal migration of the Dissection Endovascular Graft in the likely setting of an inadequate proximal landing zone (length) relative to the location of graft placement according to measurements by the core laboratory. The patient underwent a secondary intervention 131 days post-procedure to treat device separation attributed to an expanding false lumen. The patient was treated with coil embolization and stent placement.

^c Patient 1130084 had caudal migration of the Dissection Endovascular Graft in the likely setting of graft undersizing as well as an inadequate proximal landing zone (length) relative to the location of graft placement according to measurements by the core laboratory. No secondary interventions have been performed to treat this migration. The patient died 330 days post-procedure due to atherosclerotic cardiovascular disease.

^d Patient 1130044 had caudal migration of the Dissection Endovascular Graft in the likely setting of graft undersizing as well as an inadequate proximal landing zone (length) relative to the location of graft placement according to measurements by the core laboratory. No secondary interventions have been performed to treat this migration.

Table 57. Device migration in all patients based on results from core laboratory analysis and CEC confirmation

Finding	Percent Patients (number/total number)	
	6-month	12-month
Migration (> 10 mm)	6.0% (3/50)	2.2% (1/46)

Component Separation

Tables 58, 59, and 60 present data for the occurrence of component separation findings for patients who did not receive a Dissection Stent, patients who received a Dissection Stent, and the total patient population, respectively, as determined by the core laboratory. Component separation occurred in 5.9% at 6 months (2 with a Dissection Stent, 0 without a Dissection Stent) and 2.0% at 12 months (1 with a Dissection stent, 0 without a Dissection Stent). Two reports involved separation between the Dissection Endovascular Graft and Dissection Stent, while one report involved separation between two Dissection Endovascular Grafts. In each case, there appeared aortic elongation, and there were no new tears or branch vessel occlusions noted in conjunction with the separation.

Table 58. Component separation for patients who did not receive a Dissection Stent based on results from core laboratory analysis

Finding	Percent Patients (number/total number)			
	Post-procedure	1-month	6-month	12-month
Component separation	0% (0/6)	0% (0/8)	0% (0/7)	0% (0/9)

Table 59. Component separation for patients who received a Dissection Stent based on results from core laboratory analysis

Finding	Percent Patients (number/total number)			
	Post-procedure	1-month	6-month	12-month
Component separation	0% (0/30)	0% (0/40)	6.8% (3/44) ^{a,b,c}	2.5% (1/40) ^a

^a Patient 1130020 had separation between the Dissection Endovascular Graft and Dissection Stent in the setting of approximately 15 mm of apparent aortic elongation between the left common carotid and celiac (23 mm at 12 months), as compared to 11.9 mm of separation between components at 6 months (18.1 mm at 12 months).

^b Patient 1130074 had separation between the Dissection Endovascular Graft and Dissection Stent in the setting of approximately 23 mm of apparent aortic elongation between the left common carotid and celiac, as compared to 8.9 mm of separation between components.

^c Patient 1130084 had separation between two Dissection Endovascular Grafts in the setting of approximately 52 mm of apparent aortic elongation between the left common carotid and celiac, as compared to 29.5 mm of separation between components.

Table 60. Component separation for all patients based on results from core laboratory analysis

Finding	Percent Patients (number/total number)			
	Post-procedure	1-month	6-month	12-month
Component separation	0% (0/36)	0% (0/48)	5.9% (3/51)	2.0% (1/49)

Secondary Interventions

The percent of patients who required a secondary intervention within 12 months was 12.3% (9/73). This included 6.7% (1/15) of patients who did not receive a Dissection Stent and 13.8% (8/58) of patients who did receive a Dissection Stent.

Tables 61 and 62 list the patient-level details for each reintervention (days to reintervention, site-reported reasons for reintervention, and type of reintervention) for those without a Dissection Stent and those with a Dissection Stent, respectively.

Table 61. Site-reported reasons for secondary intervention in patients who did not receive a Dissection Stent

Patient	Days Post-procedure	Reason for Intervention (as reported by the site)	Type of Intervention
1130079 ^a	50	Back pain, obstruction/compromise of branch vessels, Type I proximal and distal entry-flow, and sealing re-entry tear	Three ancillary components placed and ascending aorta to innominate and LCC artery bypass

^a Patient had graft undersizing as well as an inadequate proximal landing zone (diameter and length) relative to the location of graft placement according to measurements by the core laboratory. The patient also presented with preexisting Type A dissection according to CEC adjudication.

Table 62. Site-reported reasons for secondary intervention in patients who received a Dissection Stent

Patient	Days Post-procedure	Reason for Intervention (as reported by the site)	Type of Intervention
1130006 ^a	153	Secondary entry-tear and Type I proximal entry-flow	Ascending aorta and total arch replacement; innominate, LCC artery, and LSA reconstruction

Patient	Days Post-procedure	Reason for Intervention (as reported by the site)	Type of Intervention
1130038	12	Bleeding from right groin, right femoral pseudoaneurysm	Right groin exploration with bovine patch repair of the right femoral artery
1130044 ^b	65	Secondary entry-tear just distal to the covered stent	Placement of two covered endografts
1130050	17	Pain in left arm with no signals in the left wrist; sensory slightly diminished	Left carotid to subclavian bypass and left brachial artery embolectomy
1130074 ^c	131	Device/component separation attributed to expanding false lumen	Coil embolization and stent placement
1130082 ^d	6	Right retained hemothorax	Right video-assisted thoracoscopic surgery evacuation of hematoma, decortication of right lung, flexible bronchoscopy
1130084	5	Right common iliac artery true lumen compression	Stent placement
1130086	2	Abdominal discomfort and rapid expansion of the abdominal false lumen with probable pseudoaneurysm	Coil embolization
	15	Rapidly expanding AAA, possible pseudoaneurysm	Abdominal aortic and bilateral iliac artery replacement with removal of old EVAR stent-graft system

^a Patient had graft undersizing as well as an inadequate proximal landing zone (diameter and length) relative to the location of graft placement according to measurements by the core laboratory.

^b Patient had graft undersizing as well as an inadequate proximal landing zone (length) relative to the location of graft placement according to measurements by the core laboratory.

^c Patient had separation between the Dissection Graft and Stent in the setting of approximately 23 mm of apparent aortic elongation between the left common carotid and celiac, as compared to 8.9 mm of separation between components based on the results from core lab analysis.

^d Patient had graft undersizing as well as an inadequate proximal landing zone (length) relative to the location of graft placement according to measurements by the core laboratory.

E. Post-Approval Study

Summary of the Post-Approval Study Methods

Data Source

The post-approval study for the Zenith® Dissection Endovascular System involved continued follow-up (through 5 years) of patients enrolled in the premarket pivotal clinical study that was described in Section A.

Length of Follow-up and Follow-up Rate

Long-term follow-up availability rates (2-5 years) are provided in Table 63.

Table 63. Follow-up availability (2-5 years)

Follow-up Visit	Patients Eligible for Follow-up	Percent of Data Available (Site)		Adequate Imaging to Assess the Parameter (Core Laboratory)						Events Occurring Before Next Interval				
		Clinical Assessment	CT	Size Increase in Stent-graft	Size Increase in Dissection Stent ^a	Entry-flow in Thoracic Aorta	Entry-flow in Abdominal Aorta	Migration	Device Integrity	Death	Conversion	LTF/WTHD	Other End-points ^b	Not Due for Next Visit
2-year	49	85.7% (42/49)	89.8% (44/49)	83.7% (41/49)	79.5% (31/39)	83.7% (41/49)	75.5% (37/49)	79.6% (39/49)	87.8% (43/49)	1	0	4	0	0
3-year	44	90.9% (40/44)	95.5% (42/44)	90.9% (40/44)	88.6% (31/35)	88.6% (39/44)	84.1% (37/44)	90.9% (40/44)	95.5% (42/44)	1	0	1	0	0
4-year	42	88.1% (37/42)	88.1% (37/42)	85.7% (36/42)	79.4% (27/34)	83.3% (35/42)	83.3% (35/42)	83.3% (35/42)	85.7% (36/42)	2	0	3	1	0
5-year	36	86.1% (31/36)	86.1% (31/36)	80.6% (29/36)	75.0% (21/28)	77.8% (28/36)	80.6% (29/36)	80.6% (29/36)	83.3% (30/36)	1	0	3	0	NA

NA: not assessed; LTF/WTHD: lost-to-follow-up/withdrawn.

^a Size increase in Dissection Stent assessment only applied to patients who received a Dissection Stent.^b One patient fell outside of the consented window and therefore data outside of the consented 5 years was not collected.

Summary of Final Safety and Effectiveness Findings from the Post-Approval Study (Long-term Results)

This section provides the long-term results for the following endpoints, as identified in the PMA approval order: dissection-related deaths, aortic ruptures, major adverse events (i.e., paraparesis, paraplegia, new ischemia), aortic enlargements, false lumen characteristics (i.e., diameter change, patency, and source of persistent flow), losses of device integrity, and additional dissection-related interventions, including the reasons for the interventions. No formal hypothesis testing was performed for the longer-term follow-up.

Death, Rupture, Conversion

Tables 64, 65, and 66 report the rates of death (all-cause and dissection-related), rupture, and conversion from 2-5 years in patients who did not receive a Dissection Stent, patients who received a Dissection Stent, and the total patient population, respectively. Table 67 lists the site-reported causes for each death and the results of adjudication by the CEC.

Table 64. Death, rupture, and conversion in patients who did not receive a Dissection Stent

Event	Percent Patients (number/total number)			
	366-730 Days	731-1095 Days	1096-1460 Days	1461-1825 Days
All-cause mortality	0% (0/11)	0% (0/10)	0% (0/9)	0% (0/8)
Dissection-related mortality	0% (0/11)	0% (0/10)	0% (0/9)	0% (0/8)
Rupture	0% (0/11)	0% (0/10)	0% (0/9)	0% (0/8)
Conversion	0% (0/11)	0% (0/10)	0% (0/9)	0% (0/8)

Table 65. Death, rupture, and conversion in patients who received a Dissection Stent

Event	Percent Patients (number/total number)			
	366-730 Days	731-1095 Days	1096-1460 Days	1461-1825 Days
All-cause mortality	2.2% (1/45)	2.6% (1/39)	2.9% (1/35)	9.1% (3/33)
Dissection-related mortality	0% (0/45)	0% (0/39)	0% (0/35)	0% (0/33)
Rupture	0% (0/45)	0% (0/39)	0% (0/35)	3.0% (1/33)
Conversion	2.2% (1/45)	0% (0/39)	0% (0/35)	0% (0/33)

Table 66. Death, rupture, and conversion in all patients

Event	Percent Patients (number/total number)			
	366-730 Days	731-1095 Days	1096-1460 Days	1461-1825 Days
All-cause mortality	1.8% (1/56)	2.0% (1/49)	2.3% (1/44)	7.3% (3/41)
Dissection-related mortality	0% (0/56)	0% (0/49)	0% (0/44)	0% (0/41)

Event	Percent Patients (number/total number)			
	366-730 Days	731-1095 Days	1096-1460 Days	1461-1825 Days
Rupture	0% (0/56)	0% (0/49)	0% (0/44)	2.4% (1/41)
Conversion	1.8% (1/56)	0% (0/49)	0% (0/44)	0% (0/41)

Table 67. Patient deaths

Patient Number	Days after Procedure	Dissection Stent Present (Yes/No)	Cause of Death	CEC Adjudication
1130013	454	Yes	Acute blood loss anemia and acute respiratory tract hemorrhage	Not related: related to respiratory tract hemorrhage
1130034	1291	Yes	Lung cancer	Not related: related to a preexisting condition
1130037	1816	Yes	Heart failure	Unable to be adjudicated
1130042	1589	Yes	Cardiac arrest, coronary heart disease, and congestive heart failure	Not related: related to a preexisting condition
1130050	848	Yes	Coagulopathy	Not related: related to preexisting AAA condition
1130051	1714	Yes	Metastatic cancer	Not related: related to pancreatic cancer

Major Adverse Events

Tables 68, 69, and 70 report the long-term data for the frequencies of patients experiencing MAEs in the group of patients who did not receive a Dissection Stent, the group of patients who received a Dissection Stent, and the total patient population, respectively.

Table 68. Major adverse events in patients who did not receive a Dissection Stent

Category	Percent Patients (number/total number)			
	366-730 Days	731-1095 Days	1096-1460 Days	1461-1825 Days
Myocardial infarction (includes Q-wave and non-Q-wave)	0% (0/11)	10.0% (1/10)	0% (0/9)	0% (0/8)
Renal failure requiring dialysis	0% (0/11)	0% (0/10)	0% (0/9)	0% (0/8)
Bowel ischemia	0% (0/11)	0% (0/10)	0% (0/9)	0% (0/8)
Stroke	0% (0/11)	0% (0/10)	0% (0/9)	0% (0/8)
Paraplegia	0% (0/11)	0% (0/10)	0% (0/9)	0% (0/8)
Paraparesis	0% (0/11)	0% (0/10)	0% (0/9)	0% (0/8)
Prolonged (> 72 hours) ventilatory support	0% (0/11)	0% (0/10)	0% (0/9)	0% (0/8)

Table 69. Major adverse events in patients who received a Dissection Stent

Category	Percent Patients (number/total number)			
	366-730 Days	731-1095 Days	1096-1460 Days	1461-1825 Days
Myocardial infarction (includes Q-wave and non-Q-wave)	0% (0/45)	2.6% (1/39)	0% (0/35)	0% (0/33)
Renal failure requiring dialysis	2.2% (1/45)	2.6% (1/39)	0% (0/35)	0% (0/33)
Bowel ischemia	0% (0/45)	2.6% (1/39) ^a	0% (0/35)	0% (0/33)
Stroke	2.2% (1/45)	0% (0/39)	2.9% (1/35)	0% (0/33)
Paraplegia	0% (0/45)	0% (0/39)	0% (0/35)	0% (0/33)
Paraparesis	0% (0/45)	0% (0/39)	0% (0/35)	0% (0/33)
Prolonged (> 72 hours) ventilatory support	2.2% (1/45)	2.6% (1/39)	0% (0/35)	0% (0/33)

^a Patient 1130058 experienced bowel ischemia 238 days post-procedure and 953 days post-procedure. The CEC adjudicated both events as not related, and noted that they were not convinced the patient had bowel ischemia.

Table 70. Major adverse events in all patients

Category	Percent Patients (number/total number)			
	366-730 Days	731-1095 Days	1096-1460 Days	1461-1825 Days
Myocardial infarction (includes Q-wave and non-Q-wave)	0% (0/56)	4.1% (2/49)	0% (0/44)	0% (0/41)
Renal failure requiring dialysis	1.8% (1/56)	2.0% (1/49)	0% (0/44)	0% (0/41)
Bowel ischemia	0% (0/56)	2.0% (1/49)	0% (0/44)	0% (0/41)
Stroke	1.8% (1/56)	0% (0/49)	2.3% (1/44)	0% (0/41)
Paraplegia	0% (0/56)	0% (0/49)	0% (0/44)	0% (0/41)
Paraparesis	0% (0/56)	0% (0/49)	0% (0/44)	0% (0/41)
Prolonged (> 72 hours) ventilatory support	1.8% (1/56)	2.0% (1/49)	0% (0/44)	0% (0/41)

True and False Lumen Diameter Change

Figures 4 (Dissection Stent and no Dissection Stent patients separately) and 5 (all patients combined) present the mean and standard deviation for the true lumen and false lumen diameters over time at the location of the maximum aortic diameter within the stent-graft treated segment, the Dissection Stent treated segment, and distal to the treated segment (i.e., most distal stent-graft or Dissection Stent, and within dissected aorta).

Within the stent-graft region, the average true lumen diameter increased (> 5 mm) while the average false lumen diameter decreased (> 5 mm) from post-procedure through 5-year follow-up in the total patient population as well as the groups with and without a Dissection Stent.

Within the Dissection Stent region, the average true lumen diameter increased (> 5 mm) while the average false lumen diameter remained stable ($\leq$ 5 mm change) from post-procedure through 5-year follow-up.

For the total patient population as well as the groups with and without a Dissection Stent, distal to the treated segment, the average true lumen diameter appeared stable from post-procedure through 5-year follow-up (≤ 5 mm change), whereas the average false lumen diameter appeared to increase (> 5 mm) through 5-year follow-up.

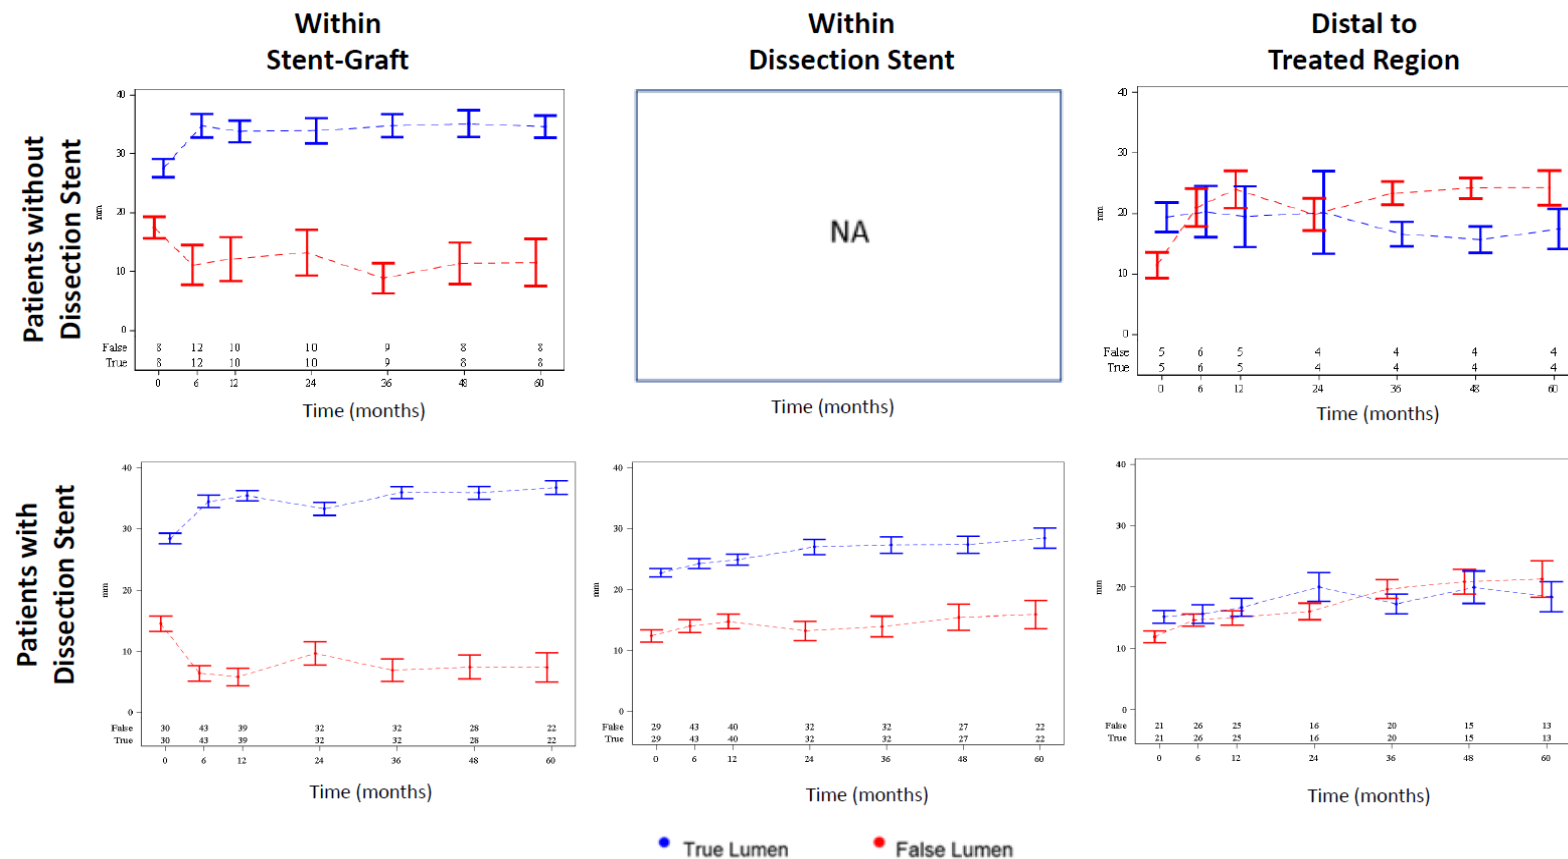


Figure 4. True and false lumen diameters over time at the location of the maximum total aortic diameter within and distal to the specified treated segments for patients who did not receive a Dissection Stent (labeled as Patients without Dissection Stent) and for patients who received a Dissection Stent (labeled as Patients with Dissection Stent). Numbers above the x-axis represent the number of patients at each time point.

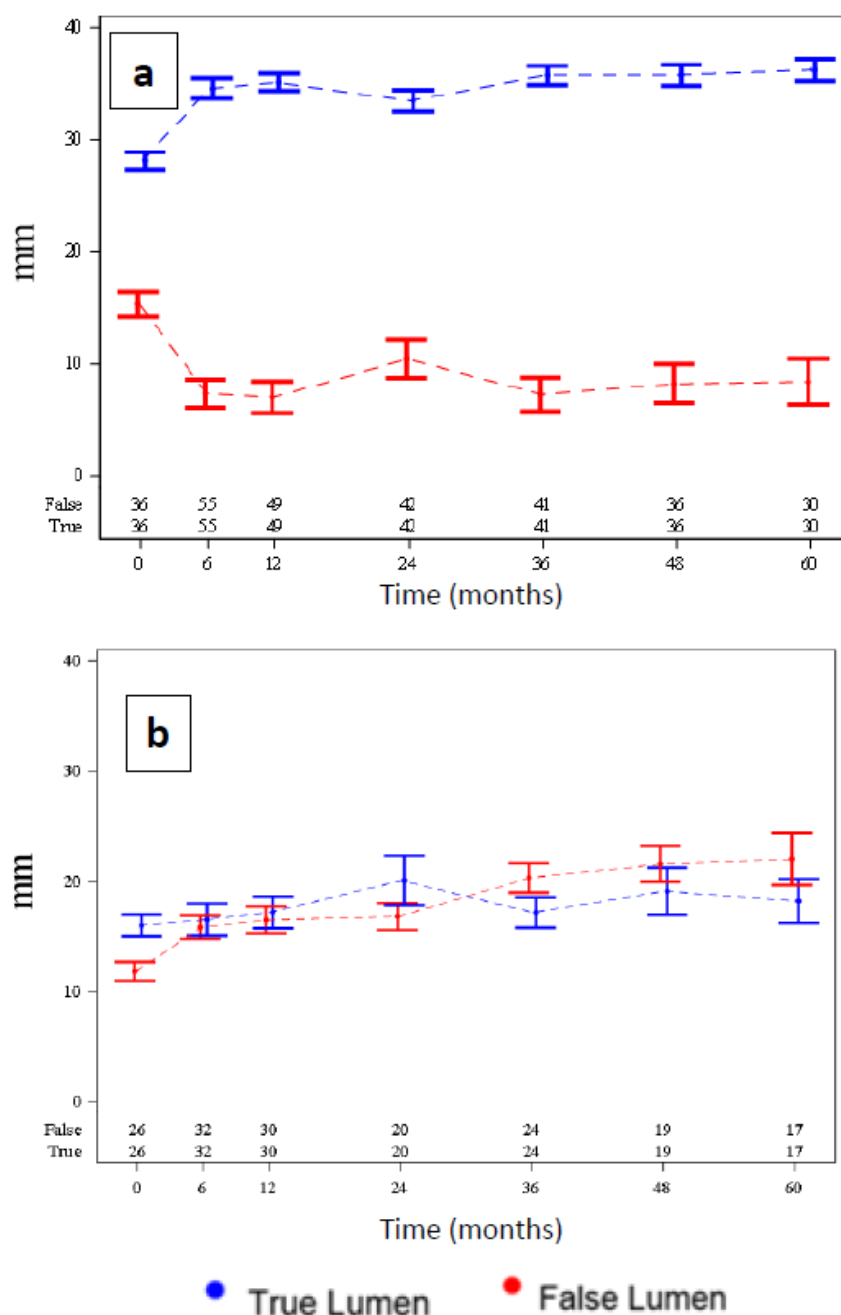


Figure 5. True and false lumen diameters over time at the location of the maximum total aortic diameter within the stent-graft (a) and distal to the treated segment (b) in the total patient population. Numbers above the x-axis represent the number of patients at each time point.

Transaortic Diameter Change in Stent-Graft Region

The results for change in transaortic diameter within the stent-graft region are presented in Tables 71, 72, and 73, which report the percentage of patients with a greater than 5 mm increase, a greater than 5 mm decrease, or no change (≤ 5 mm) in largest size in the transaortic diameter (as compared to first follow-up CT scan) within the stent-graft region for patients who did not receive a Dissection Stent, patients who received a Dissection Stent, and the total patient population, respectively, at each time point analyzed. While the focus of the post-approval study was longer-term follow-up (2-5 years), results from earlier timepoints (6 and 12 months) are reproduced below in order to demonstrate that the majority of patients with an increase in diameter during longer-term follow-up were the same patients who had an increase in diameter at earlier timepoints.

Table 71. Change in transaortic diameter within the stent-graft for patients who did not receive a Dissection Stent based on results from core laboratory analysis

Status	Percent Patients (number/total number)					
	6-month	12-month	2-year	3-year	4-year	5-year
Increase	25.0% (3/12) ^{a-c}	10.0% (1/10) ^a	20.0% (2/10) ^{a,d}	11.1% (1/9) ^a	25.0% (2/8) ^{a,c}	12.5% (1/8) ^a
Decrease	16.7% (2/12)	20.0% (2/10)	10.0% (1/10)	33.3% (3/9)	25.0% (2/8)	25.0% (2/8)
No change	58.3% (7/12)	70.0% (7/10)	70.0% (7/10)	55.6% (5/9)	50.0% (4/8)	62.5% (5/8)

^a Patient 1130081.^b Patient 1230007.^c Patient 1230010.^d Patient 1230006.^e Patient 1130027.**Table 72. Change in transaortic diameter within the stent-graft for patients who received a Dissection Stent based on results from core laboratory analysis**

Status	Percent Patients (number/total number)					
	6-month	12-month	2-year	3-year	4-year	5-year
Increase	16.3% (7/43) ^{a-g}	16.2% (6/37) ^{b-d,f,h}	25.0% (8/32) ^{a,b,d,f,h,j}	25.8% (8/31) ^{b-d,f,g,i-k}	28.6% (8/28) ^{b-f,i-k}	19.0% (4/21) ^{c,d,j,k}
Decrease	20.9% (9/43)	27.0% (10/37)	21.9% (7/32)	12.9% (4/31)	17.9% (5/28)	19.0% (4/21)
No change	62.8% (27/43)	56.8% (21/37)	53.1% (17/32)	61.3% (19/31)	53.6% (15/28)	61.9% (13/21)

^a Patient 1130017.^b Patient 1130074.^c Patient 1130006.^d Patient 1130044.^e Patient 1130057.^f Patient 1130037.^g Patient 1130052.^h Patient 1130050.ⁱ Patient 1130042.^j Patient 1130068.^k Patient 1130023.

Table 73. Change in transaortic diameter within the stent-graft for all patients based on results from core laboratory analysis

Status	Percent Patients (number/total number)					
	6-month	12-month	2-year	3-year	4-year	5-year
Increase	18.2% (10/55)	14.9% (7/47)	23.8% (10/42)	22.5% (9/40)	27.8% (10/36)	17.2% (5/29)
Decrease	20.0% (11/55)	25.5% (12/47)	19.0% (8/42)	17.5% (7/40)	19.4% (7/36)	20.7% (6/29)
No change	61.8% (34/55)	59.6% (28/47)	57.1% (24/42)	60.0% (24/40)	52.8% (19/36)	62.1% (18/29)

Transaortic Diameter Change in Dissection Stent Region

The results for change in transaortic diameter within the Dissection Stent region are presented in Table 74, which reports the percentage of patients with a greater than 5 mm increase, a greater than 5 mm decrease, or no change (≤ 5 mm) in largest size in the transaortic diameter (as compared to first follow-up CT scan) within the Dissection Stent region at each time point analyzed. While the focus of the post-approval study was longer-term follow-up (2-5 years), results from earlier timepoints (6 and 12 months) are reproduced below in order to demonstrate that the majority of patients with an increase in diameter during longer-term follow-up were the same patients who had an increase in diameter at earlier timepoints.

Table 74. Change in transaortic diameter within the Dissection Stent based on results from core laboratory analysis

Status	Percent Patients (number/total number)					
	6-month	12-month	2-year	3-year	4-year	5-year
Increase	20.5% (9/44) ^{a-i}	38.5% (15/39) ^{d-r}	45.2% (14/31) ^{b,c,h-n,p,s-v}	58.1% (18/31) ^{d-l,n-p,s-u,w-y}	59.3% (16/27) ^{b,d-l,n,p,s,x-z}	61.9% (13/21) ^{b,d,e,h,j-l,n,p,s,u,x,aa}
Decrease	4.5% (2/44)	5.1% (2/39)	6.5% (2/31)	6.5% (2/31)	3.7% (1/27)	4.8% (1/21)
No change	75.0% (33/44)	56.4% (22/39)	48.4% (15/31)	35.5% (11/31)	37.0% (10/27)	33.3% (7/21)

^a Patient 1130020.^b Patient 1130007.^c Patient 1130017.^d Patient 1130035.^e Patient 1130038.^f Patient 1130085.^g Patient 1130074.^h Patient 1130086.ⁱ Patient 1130037.^j Patient 1130006.^k Patient 1130043.^l Patient 1130064.^m Patient 1130069.ⁿ Patient 1130002.

- ^o Patient 1130057.
^p Patient 1130023.
^q Patient 1130070.
^r Patient 1130058.
^s Patient 1130008.
^t Patient 1130042.
^u Patient 1130048.
^v Patient 1130062.
^w Patient 1130025.
^x Patient 1130068.
^y Patient 1130051.
^z Patient 1130063.
^{aa} Patient 1130071.

Transaortic Diameter Change Distal To Treated Segment

The results for change in transaortic diameter distal to the treated segment and within dissected aorta are presented in Tables 75, 76, and 77, which report the percentage of patients with a greater than 5 mm increase, a greater than 5 mm decrease, or no change (≤ 5 mm) in largest size in the transaortic diameter (as compared to first follow-up CT scan) distal to the treated segment for patients who did not receive a Dissection Stent, patients who received a Dissection Stent, and the total patient population, respectively, at each time point analyzed. While the focus of the post-approval study was longer-term follow-up (2-5 years), results from earlier timepoints (6 and 12 months) are reproduced below in order to demonstrate that the majority of patients with an increase in diameter during longer-term follow-up were the same patients who had an increase in diameter at earlier timepoints.

Table 75. Change in transaortic diameter distal to the treated segment and within dissected aorta for patients who did not receive a Dissection Stent based on results from core laboratory analysis

Status	Percent Patients (number/total number)					
	6-month	12-month	2-year	3-year	4-year	5-year
Increase	16.7% (1/6) ^a	60.0% (3/5) ^{a-c}	50.0% (2/4) ^{b,c}	100% (3/3) ^{a-c}	100% (3/3) ^{a,b,c}	100% (3/3) ^{a,b,c}
Decrease	0% (0/6)	0% (0/5)	0% (0/4)	0% (0/3)	0% (0/3)	0% (0/3)
No change	83.3% (5/6)	40.0% (2/5)	50.0% (2/4)	0% (0/3)	0% (0/3)	0% (0/3)

^a Patient 1230010.

^b Patient 1130027.

^c Patient 1130081.

Table 76. Change in transaortic diameter distal to the treated segment and within dissected aorta for patients who received a Dissection Stent based on results from core laboratory analysis

Status	Percent Patients (number/total number)					
	6-month	12-month	2-year	3-year	4-year	5-year
Increase	13.0% (3/23) ^{a-c}	36.4% (8/22) ^{a-h}	50.0% (7/14) ^{b,g-l}	82.4% (14/17) ^{a-c,e-o}	92.3% (12/13) ^{a,b,e-n}	70.0% (7/10) ^{a,e,g,i,j,l,m}
Decrease	0% (0/23)	0% (0/22)	0% (0/14)	0% (0/17)	0% (0/13)	0% (0/10)
No change	87.0% (20/23)	63.6% (14/22)	50.0% (7/14)	17.6% (3/17)	7.7% (1/13)	30.0% (3/10)

^a Patient 1130076.^b Patient 1130037.^c Patient 1130052.^d Patient 1130058.^e Patient 1130038.^f Patient 1130085.^g Patient 1130043.^h Patient 1130089.ⁱ Patient 1130006.^j Patient 1130023.^k Patient 1130063.^l Patient 1130064.^m Patient 1130044.ⁿ Patient 1130047.^o Patient 1130074.**Table 77. Change in transaortic diameter distal to the treated segment and within dissected aorta for all patients based on results from core laboratory analysis**

Status	Percent Patients (number/total number)					
	6-month	12-month	2-year	3-year	4-year	5-year
Increase	13.8% (4/29)	40.7% (11/27)	50.0% (9/18)	85.0% (17/20)	93.8% (15/16)	76.9% (10/13)
Decrease	0% (0/29)	0% (0/27)	0% (0/18)	0% (0/20)	0% (0/16)	0% (0/13)
No change	86.2% (25/29)	59.3% (16/27)	50.0% (9/18)	15.0% (3/20)	6.3% (1/16)	23.1% (3/13)

False Lumen Status Within Stent-Graft Region

Tables 78, 79, and 80 present data for false lumen status within the stent-graft region for patients who did not receive a Dissection Stent, patients who received a Dissection Stent, and the total patient population, respectively. Figure 6 provides a visual representation of the data. While the focus of the post-approval study was longer-term follow-up (2-5 years), results from earlier timepoints are reproduced below in order to assist in evaluating changes in false lumen patency status over time.

Table 78. Status of false lumen within the stent-graft for patients who did not receive a Dissection Stent based on results from core laboratory analysis

Status	Percent Patients (number/total number)							
	Post-procedure	1-month	6-month	12-month	2-year	3-year	4-year	5-year
Patent	0% (0/7)	8.3% (1/12) ^a	0% (0/10)	0% (0/9)	0% (0/9)	0% (0/8)	0% (0/7)	0% (0/7)
Partially thrombosed	57.1% (4/7)	41.7% (5/12)	50.0% (5/10)	55.6% (5/9)	55.6% (5/9)	37.5% (3/8)	28.6% (2/7)	42.9% (3/7)
Completely thrombosed	42.9% (3/7)	50.0% (6/12)	40.0% (4/10)	33.3% (3/9)	33.3% (3/9)	50.0% (4/8)	71.4% (5/7)	57.1% (4/7)
No apparent false lumen	0% (0/7)	0% (0/12)	10.0% (1/10)	11.1% (1/9)	11.1% (1/9)	12.5% (1/8)	0% (0/7)	0% (0/7)

^a Patient 1230010 had false lumen flow through a secondary tear in the descending thoracic aorta as well as collateral vessels reported at 1 month; the false lumen in the stent-graft region was partially thrombosed at 6 months, 12 months, and 2 years, and was completely thrombosed at 3, 4, and 5 years.

Table 79. Status of false lumen within the stent-graft for patients who received a Dissection Stent based on results from core laboratory analysis

Status	Percent Patients (number/total number)							
	Post-procedure	1-month	6-month	12-month	2-year	3-year	4-year	5-year
Patent	0% (0/28)	0% (0/36)	0% (0/41)	0% (0/37)	0% (0/31)	0% (0/30)	0% (0/27)	0% (0/21)
Partially thrombosed	46.4% (13/28)	41.7% (15/36)	29.3% (12/41)	13.5% (5/37)	19.4% (6/31)	20.0% (6/30)	11.1% (3/27)	9.5% (2/21)
Completely thrombosed	53.6% (15/28)	52.8% (19/36)	61.0% (25/41)	78.4% (29/37)	71.0% (22/31)	66.7% (20/30)	77.8% (21/27)	81.0% (17/21)
No apparent false lumen	0% (0/28)	5.6% (2/36)	9.8% (4/41)	8.1% (3/37)	9.7% (3/31)	13.3% (4/30)	11.1% (3/27)	9.5% (2/21)

Table 80. Status of false lumen within the stent-graft for all patients based on results from core laboratory analysis

Status	Percent Patients (number/total number)							
	Post-procedure	1-month	6-month	12-month	2-year	3-year	4-year	5-year
Patent	0% (0/35)	2.1% (1/48)	0% (0/51)	0% (0/46)	0% (0/40)	0% (0/38)	0% (0/34)	0% (0/28)
Partially thrombosed	48.6% (17/35)	41.7% (20/48)	33.3% (17/51)	21.7% (10/46)	27.5% (11/40)	23.7% (9/38)	14.7% (5/34)	17.9% (5/28)
Completely thrombosed	51.4% (18/35)	52.1% (25/48)	56.9% (29/51)	69.6% (32/46)	62.5% (25/40)	63.2% (24/38)	76.5% (26/34)	75.0% (21/28)
No apparent false lumen	0% (0/35)	4.2% (2/48)	9.8% (5/51)	8.7% (4/46)	10.0% (4/40)	13.2% (5/38)	8.8% (3/34)	7.1% (2/28)

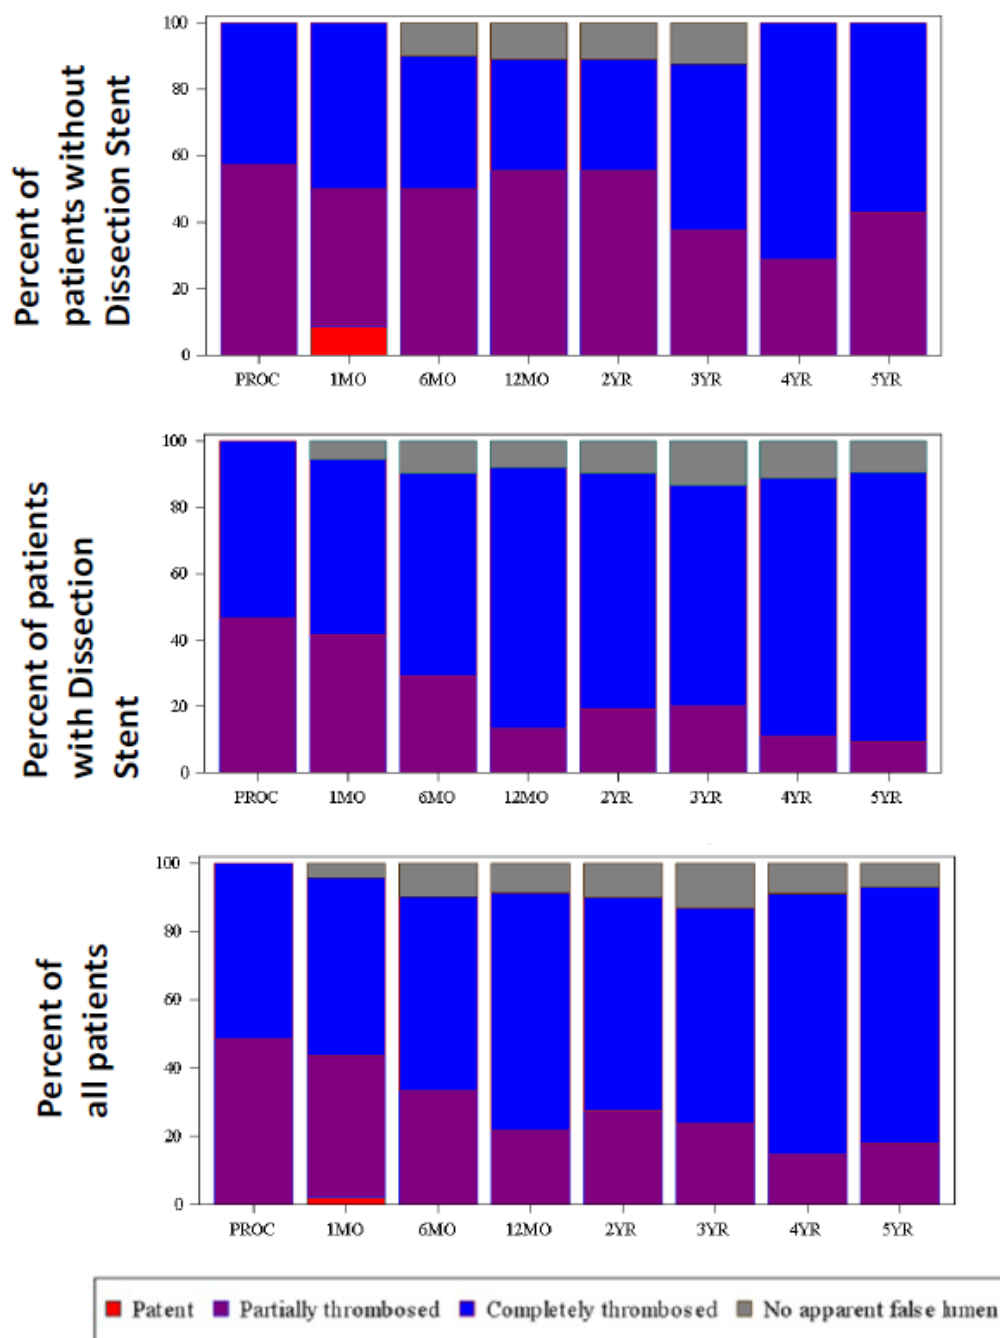


Figure 6. False lumen status within the stent-graft region for patients who did not receive a Dissection Stent (labeled as patients without Dissection Stent), patients who received a Dissection Stent (labeled as patients with Dissection Stent), and the total patient population

False Lumen Status Within The Dissection Stent Region

Table 81 presents for false lumen status within the Dissection Stent region for the patients who received a Dissection Stent at the time of the index procedure. Figure 7 provides a visual representation of the data. While the focus of the post-approval study was longer-term follow-up (2-5 years), results from earlier timepoints are reproduced below in order to assist in evaluating changes in false lumen patency status over time.

Table 81. Status of false lumen within the Dissection Stent based on results from core laboratory analysis

Status	Percent Patients (number/total number)							
	Post-procedure	1-month	6-month	12-month	2-year	3-year	4-year	5-year
Patent	10.7% (3/28) ^{a,b,c}	11.1% (4/36) ^{c-f}	2.4% (1/41) ^g	2.6% (1/39) ^h	0% (0/30)	0% (0/30)	0% (0/26)	0% (0/21)
Partially thrombosed	85.7% (24/28)	83.3% (30/36)	80.5% (33/41)	79.5% (31/39)	73.3% (22/30)	70.0% (21/30)	84.6% (22/26)	61.9% (13/21)
Completely thrombosed	3.6% (1/28)	5.6% (2/36)	14.6% (6/41)	15.4% (6/39)	16.7% (5/30)	20.0% (6/30)	11.5% (3/26)	33.3% (7/21)
No apparent false lumen	0% (0/28)	0% (0/36)	2.4% (1/41)	2.6% (1/39)	10.0% (3/30)	10.0% (3/30)	3.8% (1/26)	4.8% (1/21)

^a Patient 1130074: the false lumen in the Dissection Stent region was patent on the post-procedure CT scan; was not assessed at 1 month; was partially thrombosed at 6 months, 12 months, 2 years, 3 years, and 4 years; and could not be assessed at 5 years due to inadequate imaging.

^b Patient 1130067: the patient died 96 days post-procedure (CEC unable to adjudicate), prior to completing any additional follow-up visits.

^c Patient 1130082: the patient was lost to follow-up following the 1-month imaging.

^d Patient 1130038: the false lumen in the Dissection Stent region was partially thrombosed at 6 months, 12 months, 3 years, 4 years, and 5 years.

^e Patient 1130084: the false lumen in the Dissection Stent region was partially thrombosed at post-procedure and 6 months; the patient died 330 days post-procedure (CEC unable to adjudicate), prior to completing the 12-month follow-up visit.

^f Patient 1130057: the false lumen in the Dissection Stent region was partially thrombosed at 6 months, 12 months, 2 years, 3 years, and 4 years. The patient's 5-year visit fell outside of the consented window and therefore data were not collected.

^g Patient 1130058: the false lumen in the Dissection Stent region was partially thrombosed at post-procedure, 1 month, and 12 months. Because additional devices were implanted, the false lumen was not assessed at 2, 3, and 4 years. The patient withdrew from the study prior to the 5-year follow-up visit.

^h Patient 1130069: the false lumen in the Dissection Stent region was partially thrombosed at post-procedure, 1 month, and 2 years. The false lumen in this region was not assessed at 6 months. The patient was lost to follow-up prior to the 4-year follow-up visit.

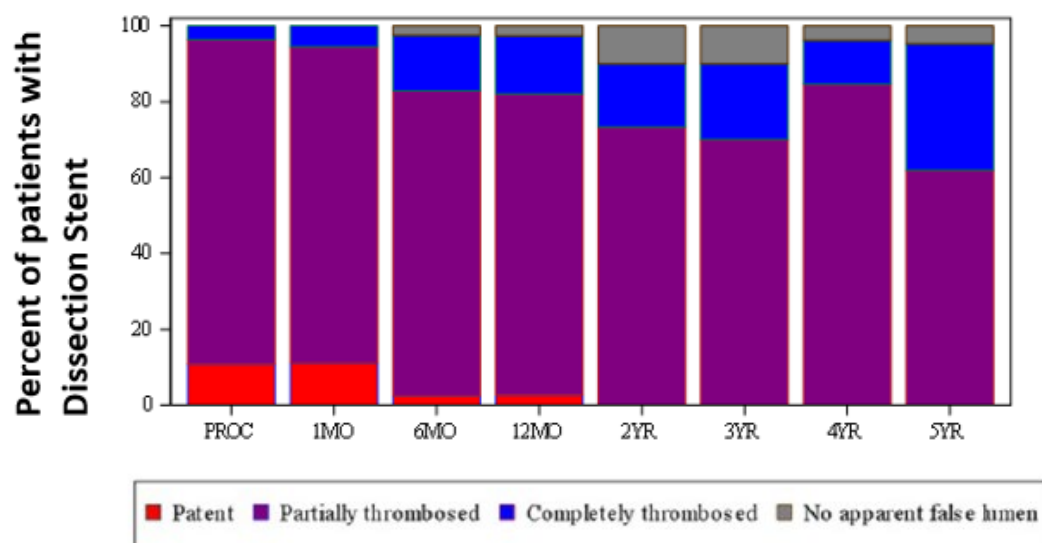


Figure 7. False lumen status within the Dissection Stent

False Lumen Status Distal To The Treated Region

Tables 82, 83, and 84 present data for false lumen status distal to the treated segment for patients who did not receive a Dissection Stent, patients who received a Dissection Stent, and the total patient population, respectively. Figure 8 provides a visual representation of the data. While the focus of the post-approval study was longer-term follow-up (2-5 years), results from earlier timepoints are reproduced below in order to assist in evaluating changes in false lumen patency status over time.

Table 82. Status of false lumen distal to the treated segment for patients who did not receive a Dissection Stent based on results from core laboratory analysis

Status	Percent Patients (number/total number)							
	Post-procedure	1-month	6-month	12-month	2-year	3-year	4-year	5-year
Patent	16.7% (1/6) ^a	16.7% (2/12) ^{b,c}	10.0% (1/10) ^a	11.1% (1/9) ^a	11.1% (1/9) ^a	12.5% (1/8) ^a	14.3% (1/7) ^a	14.3% (1/7) ^a
Partially thrombosed	33.3% (2/6)	25.0% (3/12)	40.0% (4/10)	22.2% (2/9)	22.2% (2/9)	37.5% (3/8)	42.9% (3/7)	42.9% (3/7)
Completely thrombosed	33.3% (2/6)	33.3% (4/12)	10.0% (1/10)	22.2% (2/9)	11.1% (1/9)	0% (0/8)	0% (0/7)	0% (0/7)
No apparent false lumen	16.7% (1/6)	25.0% (3/12)	40.0% (4/10)	44.4% (4/9)	55.6% (5/9)	50.0% (4/8)	42.9% (3/7)	42.9% (3/7)

^a Patient 1130081.

^b Patient 1130079.

^c Patient 1230010: partially thrombosed at subsequent time points.

Table 83. Status of false lumen distal to the treated segment for patients who received a Dissection Stent based on results from core laboratory analysis

Status	Percent Patients (number/total number)							
	Post-procedure	1-month	6-month	12-month	2-year	3-year	4-year	5-year
Patent	57.1% (16/28) ^{a-p}	25.7% (9/35) ^{i-l,o-s}	25.6% (10/39) ^{e,f,i,i,l,o,p,r,t,u,v}	18.4% (7/38) ^{b,i,p,r,s,t,w}	3.7% (1/27) ⁱ	10.0% (3/30) ^{b,i,r}	11.5% (3/26) ^{b,i,r}	5.3% (1/19) ⁱ
Partially thrombosed	21.4% (6/28)	37.1% (13/35)	48.7% (19/39)	50.0% (19/38)	63.0% (17/27)	60.0% (18/30)	50.0% (13/26)	52.6% (10/19)
Completely thrombosed	3.6% (1/28)	0% (0/35)	5.1% (2/39)	5.3% (2/38)	3.7% (1/27)	6.7% (2/30)	11.5% (3/26)	15.8% (3/19)
No apparent false lumen	17.9% (5/28)	37.1% (13/35)	20.5% (8/39)	26.3% (10/38)	29.6% (8/27)	23.3% (7/30)	26.9% (7/26)	26.3% (5/19)

^a Patient 1130047: partially thrombosed at 6 months, 1 year, 2 years, and 3 years. The patient was not assessed at 4 years or 5 years.

^b Patient 1130085.

^c Patient 1130088: partially thrombosed at subsequent time points.

^d Patient 1130066.

^e Patient 1130074: not assessed at 1 month; patent at 6 months; partially thrombosed at 12 months, 2 years, and 3 years; and completely thrombosed at 4 years. The patient was not assessed at 5 years.

^f Patient 1130087.

^g Patient 1130067.

^h Patient 1130043: partially thrombosed at subsequent time points.

ⁱ Patient 1130044.

^j Patient 1130064: partially thrombosed at subsequent time points.

^k Patient 1130082.

^l Patient 1130084.

^m Patient 1130060.

ⁿ Patient 1130052: not assessed at 1 month, partially thrombosed at 6 months and 1 year, not assessed at 2 years, partially thrombosed at 3 years, and not assessed at 4 years. The patient withdrew from the study prior to the 5-year follow up visit.

^o Patient 1130053: partially thrombosed at subsequent time points.

^p Patient 1130058: patent at post-procedure, 1 month, 6 months, and 12 months; and not assessed at 2 years, 3 years, and 4 years. The patient withdrew from the study prior to the 5-year follow-up visit.

^q Patient 1130034: patent at 1 month, not assessed at 6 months, partially thrombosed at 12 months, not assessed at 2 years, and partially thrombosed at 3 years. The patient died 1291 days post-procedure, prior to the 4-year follow up visit. The CEC adjudicated the death as not related, but related to a preexisting condition.

^r Patient 1130038: not assessed at 5 years.

^s Patient 1130013.

^t Patient 1130024.

^u Patient 1130039.

^v Patient 1130035: partially thrombosed at 1 year, not assessed at 2 years, and partially thrombosed at 4 years and 5 years.

^w Patient 1130068: not assessed at post-procedure, 1 month, and 6 months; patent at 12 months; not assessed at 2 years and 3 years; partially thrombosed at 4 years; and not assessed at 5 years.

Table 84. Status of false lumen distal to the treated segment for all patients based on results from core laboratory analysis

Status	Percent Patients (number/total number)							
	Post-procedure	1-month	6-month	12-month	2-year	3-year	4-year	5-year
Patent	50.0% (17/34)	23.4% (11/47)	22.4% (11/49)	17.0% (8/47)	5.6% (2/36)	10.5% (4/38)	12.1% (4/33)	7.7% (2/26)
Partially thrombosed	23.5% (8/34)	34.0% (16/47)	46.9% (23/49)	44.7% (21/47)	52.8% (19/36)	55.3% (21/38)	48.5% (16/33)	50.0% (13/26)
Completely thrombosed	8.8% (3/34)	8.5% (4/47)	6.1% (3/49)	8.5% (4/47)	5.6% (2/36)	5.3% (2/38)	9.1% (3/33)	11.5% (3/26)
No apparent false lumen	17.6% (6/34)	34.0% (16/47)	24.5% (12/49)	29.8% (14/47)	36.1% (13/36)	28.9% (11/38)	30.3% (10/33)	30.8% (8/26)

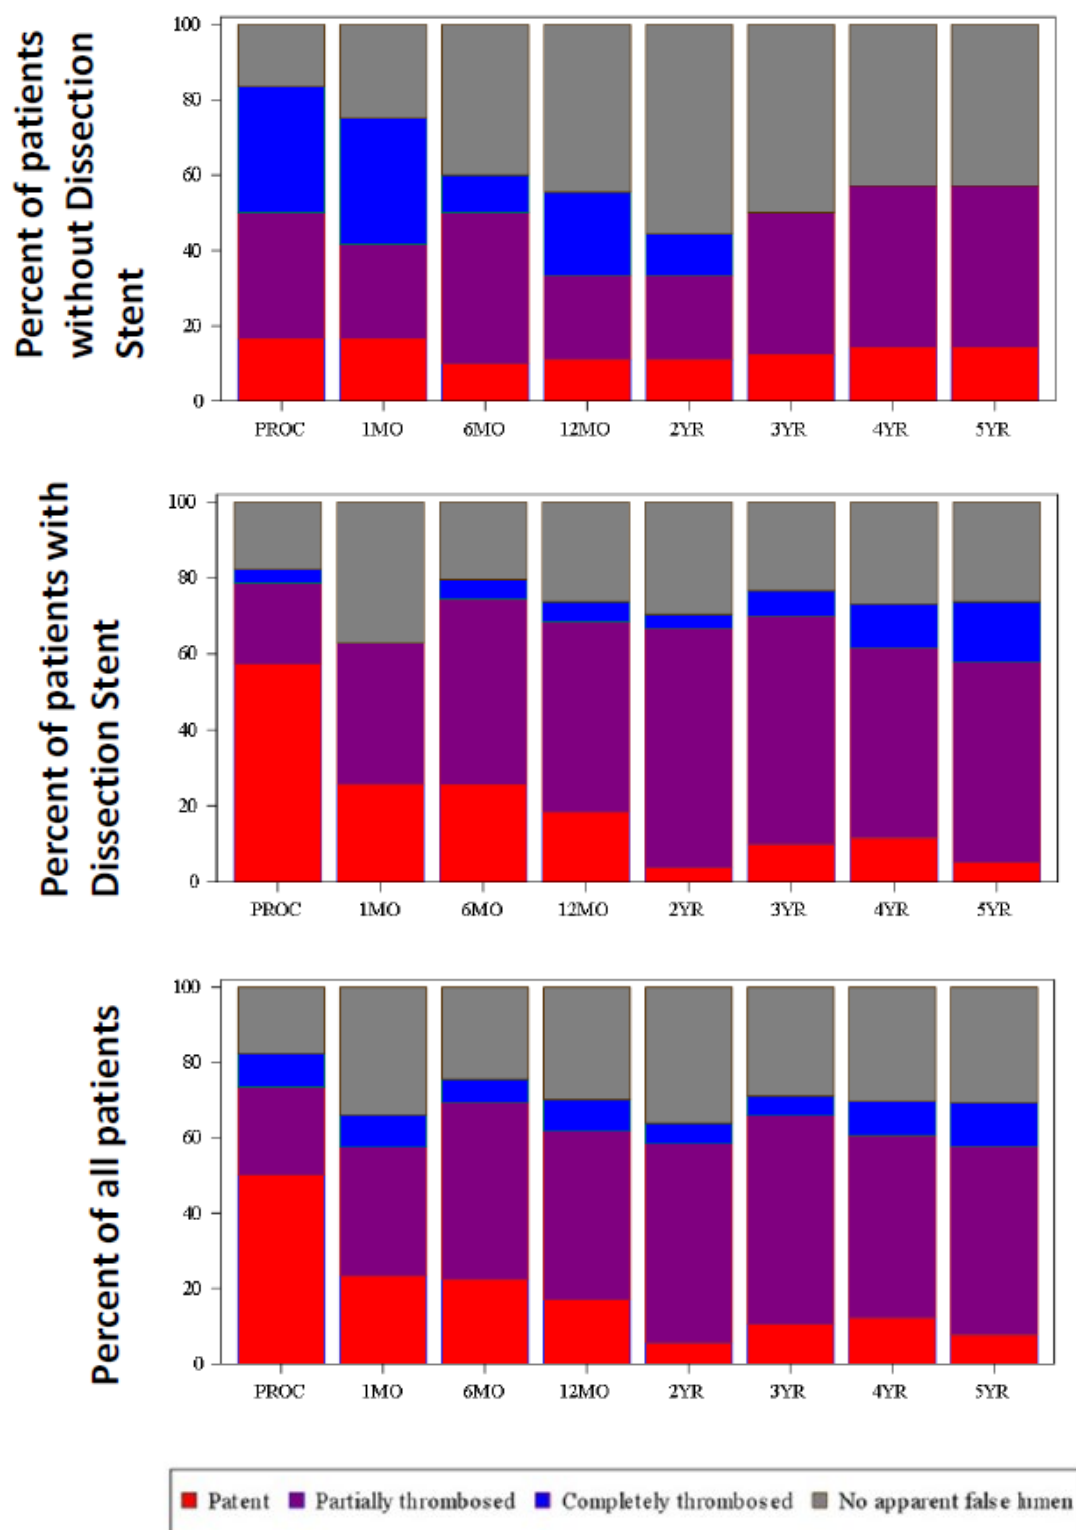


Figure 8. False lumen status distal to the treated segment for patients who did not receive a Dissection Stent (labeled as patients without Dissection Stent), patients who received a Dissection Stent (labeled as patients with Dissection Stent), and the total patient population

Source of False Lumen Flow in Thoracic Aorta

Tables 85, 86, and 87 detail sources of false lumen flow in the thoracic aorta in patients who did not receive a Dissection Stent, patients who received a Dissection Stent, and the total patient population, respectively. While the focus of the post-approval study was longer-term follow-up (2-5 years), results from earlier timepoints are reproduced below in order to demonstrate that the majority of patients with Type I endoleak during longer-term follow-up were the same patients who had Type I endoleak at earlier timepoints.

Table 85. Entry-flow in the thoracic aorta for patients who did not receive a Dissection Stent based on results from core laboratory analysis

Source	Percent Patients (number/total number)							
	Post-procedure	1-month	6-month	12-month	2-year	3-year	4-year	5-year
Multiple	14.3% (1/7)	25.0% (3/12)	10.0% (1/10)	11.1% (1/9)	22.2% (2/9)	12.5% (1/8)	14.3% (1/7)	14.3% (1/7)
Type I proximal	0% (0/7)	8.3% (1/12) ^a	10.0% (1/10) ^b	11.1% (1/9) ^b	33.3% (3/9) ^{b-d}	25.0% (2/8) ^{c,d}	14.3% (1/7) ^d	0% (0/7)
Type I distal	0% (0/7)	0% (0/12)	0% (0/10)	0% (0/9)	0% (0/9)	0% (0/8)	0% (0/7)	0% (0/7)
Type II	0% (0/7)	0% (0/12)	0% (0/10)	0% (0/9)	0% (0/9)	0% (0/8)	0% (0/7)	0% (0/7)
Type III	0% (0/7)	0% (0/12)	0% (0/10)	0% (0/9)	0% (0/9)	0% (0/8)	0% (0/7)	0% (0/7)
Type IV	0% (0/7)	0% (0/12)	0% (0/10)	0% (0/9)	0% (0/9)	0% (0/8)	0% (0/7)	0% (0/7)
Type unknown	0% (0/7)	0% (0/12)	0% (0/10)	0% (0/9)	0% (0/9)	0% (0/8)	0% (0/7)	0% (0/7)
Collateral	57.1% (4/7)	41.7% (5/12)	40.0% (4/10)	44.4% (4/9)	44.4% (4/9)	25.0% (2/8)	28.6% (2/7)	28.6% (2/7)
Secondary tear	14.3% (1/7)	33.3% (4/12)	10.0% (1/10)	11.1% (1/9)	11.1% (1/9)	12.5% (1/8)	14.3% (1/7)	14.3% (1/7)
Total patients	57.1% (4/7)	50.0% (6/12)	50.0% (5/10)	44.4% (4/9)	66.7% (6/9)	50.0% (4/8)	42.9% (3/7)	28.6% (2/7)

^a Patient 1130079 had a Type I proximal entry-flow noted at 1 month in the likely setting of graft undersizing as well as an inadequate proximal landing zone (diameter and length) relative to the location of graft placement according to measurements by the core laboratory. The patient was treated with ancillary devices and surgical bypass (Table 61) to mitigate the entry-flow. The patient also presented with preexisting Type A dissection according to CEC adjudication.

^b Patient 1130081 had a Type I proximal entry-flow first noted at 54 days post-procedure (unscheduled visit) in the likely setting of an inadequate proximal landing zone (length) relative to the location of graft placement according to measurements by the core laboratory. This entry-flow has persisted through 2 years. No secondary interventions have been performed at this time to treat this entry-flow.

^c Patient 1130040 had a Type I proximal entry-flow first noted at 2 years (also with migration at 3 years) in the likely setting of an inadequate proximal landing zone (length) relative to the location of graft placement according to measurements by the core laboratory. The entry-flow persisted at 3 years and was completely thrombosed at 4 years and 5 years.

^d Patient 1230003 had a Type I proximal entry-flow (and migration) first noted at 2 years; the dissection extended to Zone 0 at pre-procedure and thus the patient had an inadequate proximal landing zone. There has been no change since 2-year follow-up.

Table 86. Entry-flow in the thoracic aorta for patients who received a Dissection Stent based on results from core laboratory analysis

Source	Percent Patients (number/total number)							
	Post-procedure	1-month	6-month	12-month	2-year	3-year	4-year	5-year
Multiple	35.7% (10/28)	16.2% (6/37)	26.8% (11/41)	15.8% (6/38)	12.5% (4/32)	25.8% (8/31)	10.7% (3/28)	9.5% (2/21)
Type I proximal	3.6% (1/28) ^a	8.1% (3/37) ^{b-d}	4.9% (2/41) ^{a,c}	5.3% (2/38) ^{c,e}	6.3% (2/32) ^{c,e}	0% (0/31)	0% (0/28)	0% (0/21)
Type I distal	0% (0/28)	0% (0/37)	0% (0/41)	0% (0/38)	0% (0/32)	0% (0/31)	0% (0/28)	0% (0/21)
Type II	0% (0/28)	0% (0/37)	0% (0/41)	0% (0/38)	0% (0/32)	0% (0/31)	0% (0/28)	0% (0/21)
Type III	0% (0/28)	0% (0/37)	0% (0/41)	0% (0/38)	0% (0/32)	0% (0/31)	0% (0/28)	0% (0/21)
Type IV	0% (0/28)	0% (0/37)	0% (0/41)	0% (0/38)	0% (0/32)	0% (0/31)	0% (0/28)	0% (0/21)
Type unknown	0% (0/28)	2.7% (1/37)	2.4% (1/41)	2.6% (1/38)	3.1% (1/32)	3.2% (1/31)	0% (0/28)	0% (0/21)
Collateral	57.1% (16/28)	43.2% (16/37)	41.5% (17/41)	36.8% (14/38)	34.4% (11/32)	38.7% (12/31)	17.9% (5/28)	14.3% (3/21)
Secondary tear	39.3% (11/28)	27.0% (10/37)	34.1% (14/41)	18.4% (7/38)	15.6% (5/32)	29.0% (9/31)	21.4% (6/28)	19.0% (4/21)
Total patients	64.3% (18/28)	62.2% (23/37)	51.2% (21/41)	47.4% (18/38)	43.8% (14/32)	41.9% (13/31)	28.6% (8/28)	23.8% (5/21)

^a Patient 1130087 had a Type I proximal entry-flow noted at post-procedure and at 6 months in the likely setting of an inadequate proximal landing zone (length) relative to the location of graft placement according to measurements by the core laboratory. The patient died 306 days post-procedure (CEC unable to adjudicate) with no secondary interventions performed to treat this entry-flow.

^b Patient 1130025 had a Type I proximal entry-flow noted at 1 month in the likely setting of graft undersizing as well as an inadequate proximal landing zone (diameter and length) relative to the location of graft placement according to measurements by the core laboratory. The endoleak was completely resolved at 6 months without the need for reintervention.

^c Patient 1130006 had a Type I proximal entry-flow first noted at 1 month in the likely setting of graft undersizing as well as an inadequate proximal landing zone (diameter and length) relative to the location of graft placement according to measurements by the core laboratory. The patient was treated with surgical repair involving the ascending aorta and arch (Table 62). The Type I proximal entry-flow has persisted through 2 years, but resolved by 3 years.

^d Patient 1130082 had a Type I proximal entry-flow noted at 1 month, in the likely setting of graft undersizing as well as an inadequate proximal landing zone (length) relative to the location of graft placement according to measurements by the core laboratory. No secondary interventions have been performed to treat this entry-flow and the patient was reported lost to follow-up subsequent to the 1-month visit.

^e Patient 1130044 had a Type I proximal entry-flow noted at 12 months, in the likely setting of graft undersizing as well as an inadequate proximal landing zone (length) relative to the location of graft placement according to measurements by the core laboratory. The Type I proximal entry-flow persisted at 2 years but was completely resolved by 3 years.

Table 87. Entry-flow in the thoracic aorta for all patients based on results from core laboratory analysis

Source	Percent Patients (number/total number)							
	Post-procedure	1-month	6-month	12-month	2-year	3-year	4-year	5-year
Multiple	31.4% (11/35)	18.4% (9/49)	23.5% (12/51)	14.9% (7/47)	14.6% (6/41)	23.1% (9/39)	11.4% (4/35)	10.7% (3/28)
Type I proximal	2.9% (1/35)	8.2% (4/49)	5.9% (3/51)	6.4% (3/47)	12.2% (5/41)	5.1% (2/39)	2.9% (1/35)	0% (0/28)
Type I distal	0% (0/35)	0% (0/49)	0% (0/51)	0% (0/47)	0% (0/41)	0% (0/39)	0% (0/35)	0% (0/28)
Type II	0% (0/35)	0% (0/49)	0% (0/51)	0% (0/47)	0% (0/41)	0% (0/39)	0% (0/35)	0% (0/28)
Type III	0% (0/35)	0% (0/49)	0% (0/51)	0% (0/47)	0% (0/41)	0% (0/39)	0% (0/35)	0% (0/28)

Source	Percent Patients (number/total number)							
	Post-procedure	1-month	6-month	12-month	2-year	3-year	4-year	5-year
Type IV	0% (0/35)	0% (0/49)	0% (0/51)	0% (0/47)	0% (0/41)	0% (0/39)	0% (0/35)	0% (0/28)
Type unknown	0% (0/35)	2.0% (1/49)	2.0% (1/51)	2.1% (1/47)	2.4% (1/41)	2.6% (1/39)	0% (0/35)	0% (0/28)
Collateral	57.1% (20/35)	42.9% (21/49)	41.2% (21/51)	38.3% (18/47)	36.6% (15/41)	35.9% (14/39)	20.0% (7/35)	17.9% (5/28)
Secondary tear	34.3% (12/35)	28.6% (14/49)	29.4% (15/51)	17.0% (8/47)	14.6% (6/41)	25.6% (10/39)	20.0% (7/35)	17.9% (5/28)
Total patients	62.9% (22/35)	59.2% (29/49)	51.0% (26/51)	46.8% (22/47)	48.8% (20/41)	43.6% (17/39)	31.4% (11/35)	25.0% (7/28)

Source of False Lumen Flow in Abdominal Aorta

Tables 88, 89, and 90 detail sources of entry-flow in the abdominal aorta in the patients who did not receive a Dissection Stent, patients who received a Dissection Stent, and the total patient population, respectively. As with previous sections, results from earlier time points are reproduced below for reference.

Table 88. Entry-flow in the abdominal aorta for patients who did not receive a Dissection Stent based on results from core laboratory analysis

Source	Percent Patients (number/total number)							
	Post-procedure	1-month	6-month	12-month	2-year	3-year	4-year	5-year
Multiple	28.6% (2/7)	20.0% (2/10)	22.2% (2/9)	33.3% (2/6)	28.6% (2/7)	33.3% (2/6)	42.9% (3/7)	42.9% (3/7)
Type I proximal	0% (0/7)	0% (0/10)	0% (0/9)	0% (0/6)	0% (0/7)	0% (0/6)	0% (0/7)	0% (0/7)
Type I distal	0% (0/7)	0% (0/10)	0% (0/9)	0% (0/6)	0% (0/7)	0% (0/6)	0% (0/7)	0% (0/7)
Type II	0% (0/7)	0% (0/10)	0% (0/9)	0% (0/6)	0% (0/7)	0% (0/6)	0% (0/7)	0% (0/7)
Type III	0% (0/7)	0% (0/10)	0% (0/9)	0% (0/6)	0% (0/7)	0% (0/6)	0% (0/7)	0% (0/7)
Type IV	0% (0/7)	0% (0/10)	0% (0/9)	0% (0/6)	0% (0/7)	0% (0/6)	0% (0/7)	0% (0/7)
Type unknown	0% (0/7)	0% (0/10)	0% (0/9)	0% (0/6)	0% (0/7)	0% (0/6)	0% (0/7)	0% (0/7)
Collateral	42.9% (3/7)	40.0% (4/10)	44.4% (4/9)	33.3% (2/6)	28.6% (2/7)	33.3% (2/6)	42.9% (3/7)	42.9% (3/7)
Secondary tear	28.6% (2/7)	20.0% (2/10)	33.3% (3/9)	50.0% (3/6)	28.6% (2/7)	33.3% (2/6)	42.9% (3/7)	42.9% (3/7)
Total patients	42.9% (3/7)	40.0% (4/10)	55.6% (5/9)	50.0% (3/6)	28.6% (2/7)	33.3% (2/6)	42.9% (3/7)	42.9% (3/7)

Table 89. Entry-flow in the abdominal aorta for patients who received a Dissection Stent based on results from core laboratory analysis

Source	Percent Patients (number/total number)							
	Post-procedure	1-month	6-month	12-month	2-year	3-year	4-year	5-year
Multiple	82.1% (23/28)	70.3% (26/37)	63.2% (24/38)	66.7% (26/39)	60.0% (18/30)	66.7% (21/31)	64.3% (18/28)	59.1% (13/22)
Type I proximal	0% (0/28)	2.7% (1/37) ^a	0% (0/38)	0% (0/39)	0% (0/30)	0% (0/31)	0% (0/28)	0% (0/22)
Type I distal	0% (0/28)	0% (0/37)	0% (0/38)	0% (0/39)	0% (0/30)	0% (0/31)	0% (0/28)	0% (0/22)
Type II	0% (0/28)	0% (0/37)	0% (0/38)	0% (0/39)	0% (0/30)	0% (0/31)	0% (0/28)	0% (0/22)
Type III	0% (0/28)	0% (0/37)	0% (0/38)	0% (0/39)	0% (0/30)	0% (0/31)	0% (0/28)	0% (0/22)
Type IV	0% (0/28)	0% (0/37)	0% (0/38)	0% (0/39)	0% (0/30)	0% (0/31)	0% (0/28)	0% (0/22)
Type unknown	0% (0/28)	0% (0/37)	2.6% (1/38)	0% (0/39)	0% (0/30)	0% (0/31)	0% (0/28)	0% (0/22)
Collateral	92.9% (26/28)	81.1% (30/37)	84.2% (32/38)	76.9% (30/39)	73.3% (22/30)	77.4% (24/31)	75.0% (21/28)	72.7% (16/22)
Secondary tear	89.3% (25/28)	75.7% (28/37)	71.1% (27/38)	74.4% (29/39)	63.3% (19/30)	77.4% (24/31)	75.0% (21/28)	63.6% (14/22)
Total patients	100% (28/28)	89.2% (33/37)	92.1% (35/38)	84.6% (33/39)	76.7% (23/30)	87.1% (27/31)	85.7% (24/28)	77.3% (17/22)

^a Patient 1130006 had a Type I proximal entry-flow noted at 1 month in the likely setting of graft undersizing as well as an inadequate proximal landing zone (diameter and length) relative to the location of graft placement according to measurements by the core laboratory. The patient underwent a surgical repair involving the ascending aorta and arch 153 days post-procedure (Table 62).

Table 90. Entry-flow in the abdominal aorta for all patients based on results from core laboratory analysis

Source	Percent Patients (number/total number)							
	Post-procedure	1-month	6-month	12-month	2-year	3-year	4-year	5-year
Multiple	71.4% (25/35)	59.6% (28/47)	55.3% (26/47)	62.2% (28/45)	54.1% (20/37)	62.2% (23/37)	60.0% (21/35)	55.2% (16/29)
Type I proximal	0% (0/35)	2.1% (1/47)	0% (0/47)	0% (0/45)	0% (0/37)	0% (0/37)	0% (0/35)	0% (0/29)
Type I distal	0% (0/35)	0% (0/47)	0% (0/47)	0% (0/45)	0% (0/37)	0% (0/37)	0% (0/35)	0% (0/29)
Type II	0% (0/35)	0% (0/47)	0% (0/47)	0% (0/45)	0% (0/37)	0% (0/37)	0% (0/35)	0% (0/29)
Type III	0% (0/35)	0% (0/47)	0% (0/47)	0% (0/45)	0% (0/37)	0% (0/37)	0% (0/35)	0% (0/29)
Type IV	0% (0/35)	0% (0/47)	0% (0/47)	0% (0/45)	0% (0/37)	0% (0/37)	0% (0/35)	0% (0/29)
Type unknown	0% (0/35)	0% (0/47)	2.1% (1/47)	0% (0/45)	0% (0/37)	0% (0/37)	0% (0/35)	0% (0/29)
Collateral	82.9% (29/35)	72.3% (34/47)	76.6% (36/47)	71.1% (32/45)	64.9% (24/37)	70.3% (26/37)	68.6% (24/35)	65.5% (19/29)
Secondary tear	77.1% (27/35)	63.8% (30/47)	63.8% (30/47)	71.1% (32/45)	56.8% (21/37)	70.3% (26/37)	68.6% (24/35)	58.6% (17/29)
Total patients	88.6% (31/35)	78.7% (37/47)	85.1% (40/47)	80.0% (36/45)	67.6% (25/37)	78.4% (29/37)	77.1% (27/35)	69.0% (20/29)

Retrograde/Proximal Extension of Dissection

In total, there have been 7 patients with site-reported proximal dissection events, including 4 described by the sites as retrograde progression of dissection (1130039, 1130060, 1130068, and 1130079) and 3 described as a new tear/Type A dissection (1130001, 1130025, and 1130089); 3 patients died (each within 365 days) and 4 required reintervention (1 within 365 days, 3 after 365 days). None of the proximal dissection events were considered retrograde progression of Type B dissection to Type A dissection, as 6 patients had evidence of preexisting disease proximal to the LSA prior to study enrollment and 1 had a Type B dissection that was no longer apparent prior to developing a new Type A dissection. No additional patients with retrograde/proximal extension were identified based on core laboratory analysis.

Antegrade/Distal Extension of Dissection

In total, there have been 2 patients (1130002 and 1130088) with antegrade/distal extension of dissection (both occurrences happened within 365 days and involved patients treated with a Dissection Stent).

Device Integrity

There were no new device integrity findings (e.g., kink, stent fracture, compression, infolding) detected by the core laboratory between 2 and 5 years post-procedure.

Secondary Interventions

No secondary interventions were performed between 2 and 5 years post-procedure in patients who did not receive a Dissection Stent. Table 91 summarizes the site-reported reasons for secondary intervention between 2 and 5 years post-procedure for patients who received a Dissection Stent.

Table 91. Site-reported reasons for secondary intervention in patients who received a Dissection Stent

Reason	366-730 Days	731-1095 Days	1096-1460 Days	> 1460 Days
Aortic rupture	0	0	0	0
Device kink	0	0	0	0
Device migration	0	0	0	0
Device separation	0	0	0	0
Device stenosis	0	0	0	0
Device infection	1 ^b	0	0	0

Reason	366-730 Days	731-1095 Days	1096-1460 Days	> 1460 Days
Occlusion	0	0	0	0
Obstruction/compromise of branch vessels	0	0	1 ^a	0
Entry-flow				
Type I proximal	2 ^c	0	0	0
Type I distal	1 ^c	0	0	0
Type II	0	0	0	0
Type III (graft overlap joint)	0	0	0	0
Type III (hole/tear in graft)	0	0	0	0
Type IV (through graft body)	0	0	0	0
Unknown	0	0	0	0
Secondary tear	2 ^d	0	0	1 ^h
Collateral	1 ^d	0	0	0
Sealing re-entry tear	0	0	0	0
Other	2 ^{c,d}	2 ^{d,e}	2 ^{f,g}	0

^a Patient 1130074.^b Patient 1130090.^c Patient 1130023.^d Patient 1130058.^e Patient 1130057.^f Patient 1130025.^g Patient 1130089.^h Patient 1130068.

Table 92 summarizes the site-reported types of secondary interventions performed between 2 and 5 years post-procedure for patients who received a Dissection Stent.

Table 92. Types of secondary interventions in patients who received a Dissection Stent

Type	366-730 Days	731-1095 Days	1096-1460 Days	> 1460 Days
Percutaneous				
Ancillary component placed	3 ^{b,c}	1 ^c	0	0
Balloon angioplasty	2 ^{b,c}	0	0	0
Coil embolization	1 ^c	0	0	0
Stent	2 ^c	0	1 ^a	0
Thrombectomy	0	1 ^c	0	0
Thrombolysis	0	0	0	0
Other	0	0	1 ^a	0
Surgical				
Conversion to open repair	1 ^d	0	0	0
Surgical bypass procedure	0	0	0	0
Other	2 ^{b,c}	1 ^c	2 ^{f,g}	1 ^h
Other	0	0	0	0

^a Patient 1130074. ^b Patient 1130023.^c Patient 1130058. Note that this patient had three separate secondary interventions whereby ancillary components and/or stents were placed (see Table 93).^d Patient 1130090.^e Patient 1130057.

^f Patient 1130025.^g Patient 1130089.^h Patient 1130068.

Patient-level details for each secondary intervention between 2 and 5 years post-procedure (including timing, reason, and type) in patients who received a Dissection Stent are provided in Table 93.

Table 93. Detailed information regarding secondary intervention in patients who received a Dissection Stent

Patient	Days Post-procedure	Reason for Intervention (as reported by the site)	Type of Intervention
1130023	390	Type I proximal and distal entry-flow	Ancillary component placed and balloon angioplasty
	608	Type I proximal entry-flow and sinus of Valsalva aneurysm with aortic valve insufficiency secondary to bicuspid aortic valve	Composite aortic root replacement and total arch replacement
1130025	1161	New tear in ascending thoracic aorta and intermittent chest pressure at rest and when walking quickly	Replacement of aortic valve and ascending aorta
1130057	893	New penetrating ulcer and aneurysmal degeneration distal to the stent-grafts, but within the Dissection Stent	Ancillary component placed
1130058	530	Worsening chronic abdominal pain and chest pain, abdominal tenderness, as well as a secondary tear at the distal end of the stent-graft	Ancillary component placed and balloon angioplasty
	655	Abdominal pain, secondary tears in the distal infrarenal aorta and at the celiac artery, and collateral flow from the lumbar arteries	Ancillary components placed, stents placed, and coil embolization
	711	Bloody stools and abdominal pain, incomplete collapse of the proximal SMA stent that was deployed on September 16, 2015	Stent placed
	920	Worsening abdominal pain with radiation to the back and right thigh, paresthesia and numbness in the right leg when patient tries to walk, and thrombus in the right CFA extending into the profunda and SFA	Embolectomy and thrombectomy of the right femoropopliteal artery
1130068	1528	Acute Type A dissection with involvement of aortic arch and aneurysmal ascending aorta	Open surgical repair of Type A aortic arch dissection
1130074	1190	Lower extremity claudication, obstruction/compromise of branch vessels	Bifurcated AAA graft and iliac extension stent placed
1130089	1290	New separate Type A dissection	Ascending aortic arch replacement

Patient	Days Post-procedure	Reason for Intervention (as reported by the site)	Type of Intervention
1130090	650	Fatigue, lethargy, failure to thrive; positive blood cultures and imaging indicated an infected stent-graft	Graft explanted and patient underwent conversion to open repair

Study Strengths and Weaknesses

This clinical study was well controlled, having been conducted in accordance with ISO 14155, 21 CFR 812, JGCP, ICH GCP, and other applicable requirements as appropriate. Additionally, the study utilized an independent core laboratory to ensure uniform analysis of pre-procedure and follow-up imaging exams.

While the data were analyzed and reported separately for patients with a Dissection Stent and patients without a Dissection Stent, the study was not powered to assess for differences in outcomes based on the presence vs. absence of a Dissection Stent. Nearly one-third of patients died during follow-up (often due to preexisting conditions or other reasons unrelated to the device), thus limiting the number of enrolled patients with completed 5-year follow-up.

References

1. Fillinger MF, Greenberg RK, McKinsey JF, Chaikof EL; for the Society for Vascular Surgery Ad Hoc Committee on TEVAR Reporting Standards. Reporting standards for thoracic endovascular aortic repair (TEVAR). J Vasc Surg. 2010;52:1022-33.