


Fusion[®] OMNI[™]

SPHINCTEROTOME WITH DOMETIP[®]

Always


- 1) Lubricate the top of the Fusion Wire Guide Locking Device cap with water soluble lubricant.
- 2) Flush the wire guide lumen of the OMNI device prior to inserting the wire guide. Cover the Wire Control Port with the black slide cover or your thumb prior to flushing.

Step 1

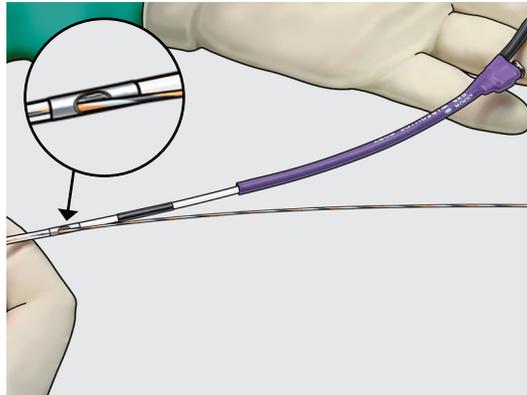


Insert the wire guide into the wire control port.

Step 2

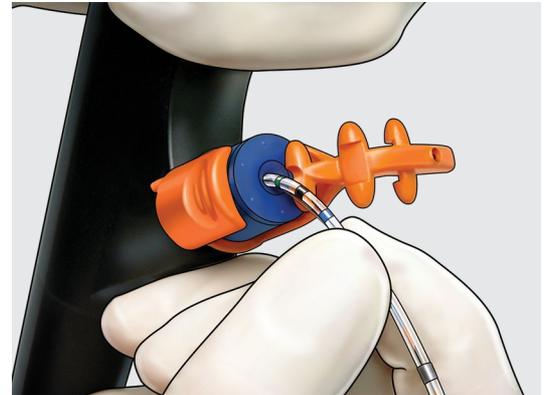


The OMNI device tip is soft. Gently put the tip into the wire lock cap so that it slides beyond the internal seal in the cap.

Step 3

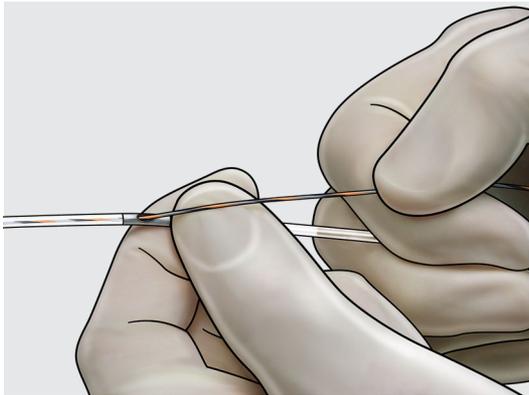


For physician wire guide control, pop and zip the wire guide down to the wire guide locking device. Hold the catheter and the wire guide in one hand and use opposite thumb to abruptly "pop" the wire guide through the breakthrough channel at the wire control port.

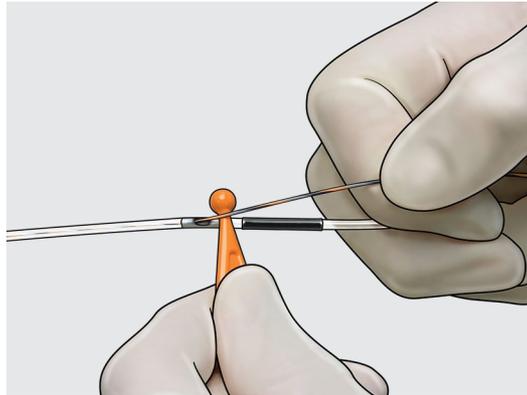


As an alternative method, use the zip tool, included with the product. Hold the catheter and the wire guide in one hand and use the zip tool to abruptly "pop" the wire guide through the breakthrough channel at the wire control port.

Step 4

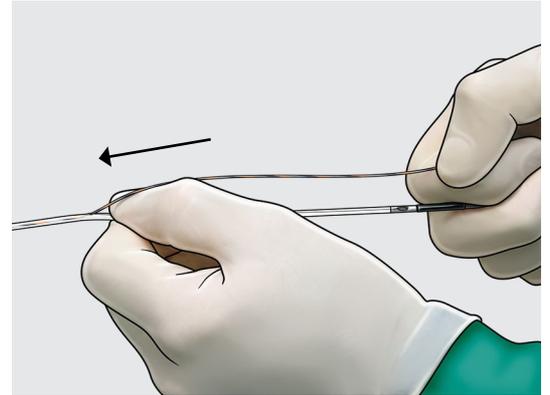


Continue to zip the wire guide out of the breakthrough channel with thumb **or** zip tool while continuing to hold the catheter and wire guide in the opposite hand.

Step 5

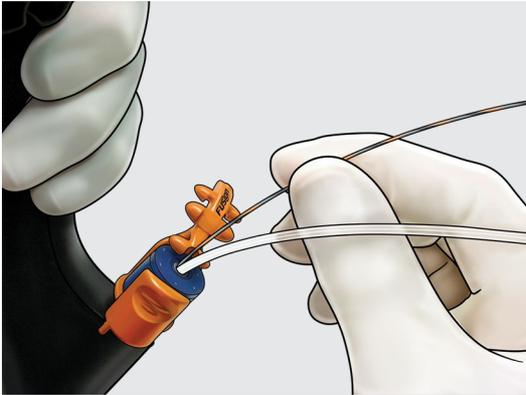


The physician now has wire guide control.

Step 6

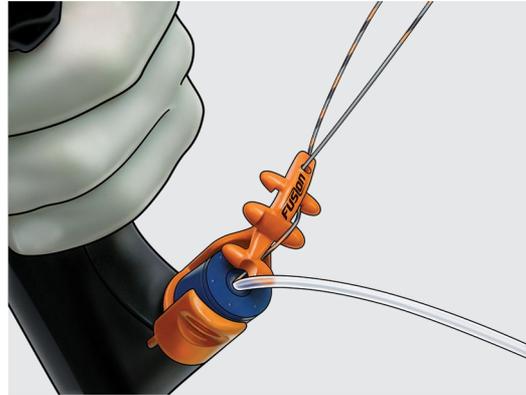


Once wire guide access is achieved, the wire should be locked to the locking device. Weave the wire guide in an "under-over-under" pattern and place the tail of the wire guide into the wire-tail port.

Step 7

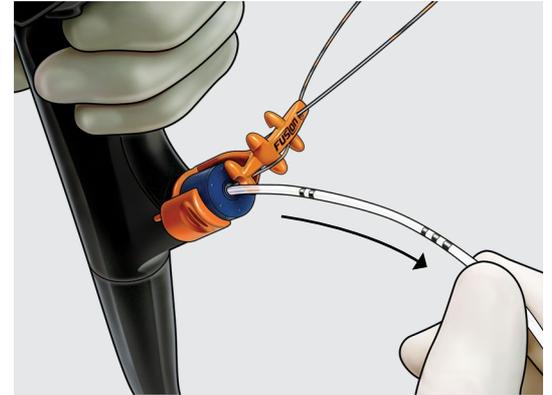


To zip the OMNI device out of the scope, ensure the elevator is **down**. Pull the device upwards out of the scope until the radiopaque band reaches the cap.

Step 8

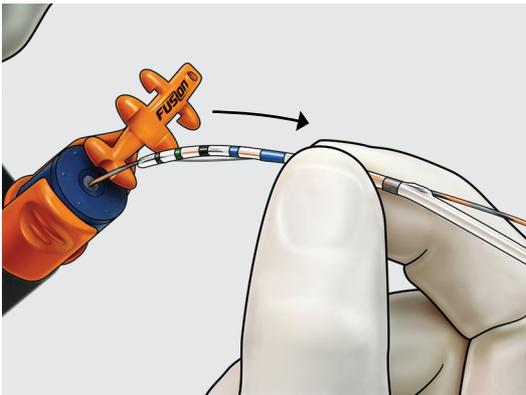

Unlock the wire guide and perform the exchange to remove the OMNI device from the wire guide.

Step 9

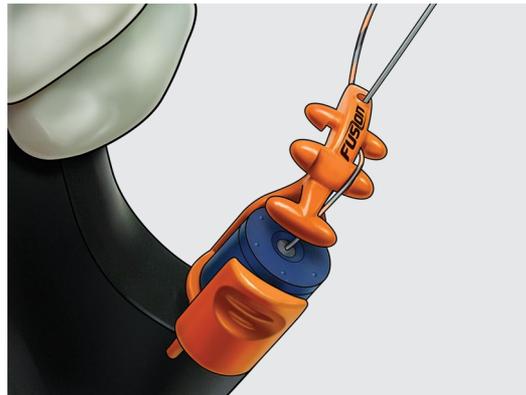

Lock the wire guide to the locking device. Weave the wire guide in an "under-over-under" pattern and place the tail of the wire guide into the wire-tail port. Proceed with the next Fusion device.

Refer to current instructions for detailed system use.

Customer Service

EU Website: cookmedical.eu
EDI: cookmedical.eu/edi
Distributors: +353 61239240, ssc.distributors@cookmedical.com
Austria: +43 179567121, oe.orders@cookmedical.com
Belgium: +32 27001633, be.orders@cookmedical.com
Denmark: +45 38487607, da.orders@cookmedical.com
Finland: +358 972519996, fi.orders@cookmedical.com
France: +33 171230269, fr.orders@cookmedical.com
Germany: +49 6950072804, de.orders@cookmedical.com
Hungary: +36 17779199, hu.orders@cookmedical.com
Ireland: +353 61239252, ie.orders@cookmedical.com
Italy: +39 0269682853, it.orders@cookmedical.com
Netherlands: +31 202013367, nl.orders@cookmedical.com
Norway: +47 23162968, no.orders@cookmedical.com
Spain: +34 912702691, es.orders@cookmedical.com
Sweden: +46 858769468, se.orders@cookmedical.com
Switzerland - French: +41 448009609, fr.orders@cookmedical.com
Switzerland - Italian: +41 448009609, it.orders@cookmedical.com
Switzerland - German: +41 448009609, de.orders@cookmedical.com
United Kingdom: +44 2073654183, uk.orders@cookmedical.com

USA Website: cookmedical.com
EDI: cookmedical.com/edi.do
Americas:
Phone: +1 812.339.2235, 800.457.4500, Fax: 800.554.8335
E-mail: orders@cookmedical.com
Australia:
Phone: +61 734346000, 1800777222, Fax: +61 734346001, 1800077283
E-mail: cau.custserv@cookmedical.com-A4



AI, ESC, IR, OHNS, PI, RH, SUR-A4