

ShortShot®

SAEED® HEMORRHOIDAL MULTI-BAND LIGATOR WITH TRIVIEW® ANOSCOPE

Equipment Needed

- Medical grade suction equipment
- Source of illumination
- Water-soluble lubricant

Preparation


Preparation of anoscope - Prior to procedure, test maneuverability of ShortShot barrel in lumen of anoscope.

Preparation of ligation bander -

1. Connect suction tube from suction unit to graduated connector at bottom of ligator handle.
2. Place finger on suction port and verify suction is present at tip of ligator barrel.
3. Ensure settings on suction unit are appropriate for suction of hemorrhoids into tip of ligator barrel.


ShortShot is now ready for ligation of hemorrhoids.

Step 1

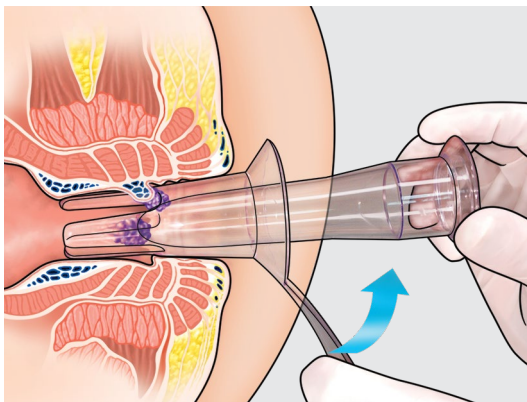

Anoscope with obturator comes assembled in package. Remove obturator from anoscope and reinsert before use to ensure proper function. Lubricate anoscope and obturator and insert them into patient's anus. Rotate anoscope in anus so handle is aligned upwards towards patient's spine.


Step 2

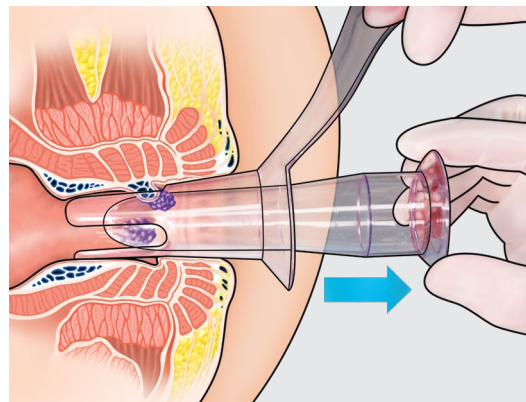

Remove obturator from anoscope and inspect lumen. Up to three internal hemorrhoids will be aligned in the three slots of anoscope. Slots are designed to coincide with anatomical location of hemorrhoids in most adults. It may be necessary to rotate anoscope a small amount in either direction to encourage any swollen hemorrhoids to fall into place.

Note: This anoscope may be used in patients with fewer than three hemorrhoids.


Step 3

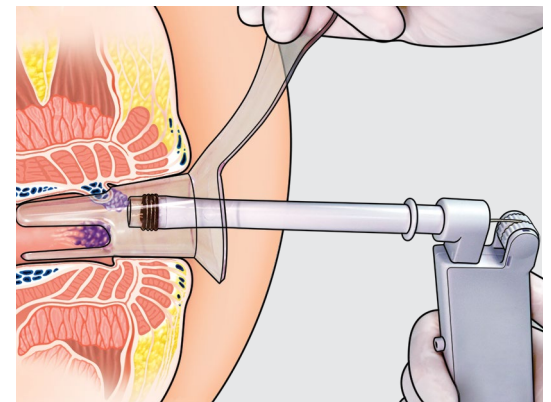

Insert ShortShot into lumen of the anoscope.


Caution: Do not cover suction port prior to achieving desired ligation position.

Step 4

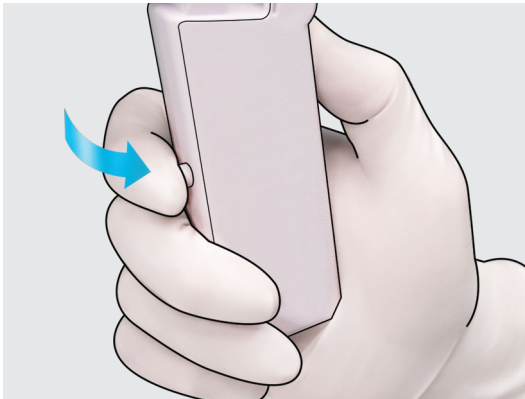

After full contact is made between barrel tip of ligator and hemorrhoid, suction hemorrhoid into ligator by covering suction port.

Step 5

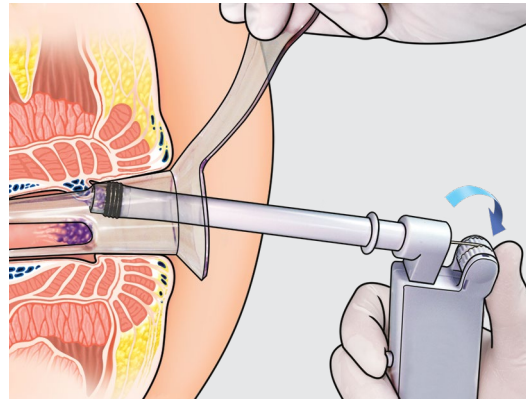

Maintain suction of hemorrhoid by keeping suction port covered. Deploy band by slowly rotating spool downward until tension is released.

Step 6

Uncover suction port of ligator to relieve suction on hemorrhoid. This will allow ligated hemorrhoid to release from tip of ShortShot. Withdraw device.

Step 7

Repeat ligation process on any remaining hemorrhoids. If more than 4 bands are required to complete treatment, use an additional ShortShot.

Step 8

Upon completion of procedure, remove ligator and anoscope from patient. It is not necessary to reinsert obturator into anoscope to remove ligator and anoscope.

Step 9

Dispose of ShortShots per institutional guidelines for biohazardous medical waste.

Please refer to the product's Instructions for Use (IFU) for full prescribing information, warnings, precautions, contraindications, and potential adverse events.

Customer Service

EU Website: cookmedical.eu
EDI: cookmedical.eu/edi
Distributors: +353 61239240, ssc.distributors@cookmedical.com
Austria: +43 179567121, oe.orders@cookmedical.com
Belgium: +32 27001702, be.orders@cookmedical.com
Denmark: +45 38487607, da.orders@cookmedical.com
Finland: +358 972519996, fi.orders@cookmedical.com
France: +33 171230269, fr.orders@cookmedical.com
Germany: +49 6950072804, de.orders@cookmedical.com
Hungary: +36 17779199, hu.orders@cookmedical.com
Iceland: +354 8007615, IS.orders@cookmedical.com
Ireland: +353 61239252, ie.orders@cookmedical.com
Italy: +39 0269682853, it.orders@cookmedical.com
Netherlands: +31 202013367, nl.orders@cookmedical.com
Norway: +47 23162968, no.orders@cookmedical.com
Spain: +34 912702691, es.orders@cookmedical.com
Sweden: +46 858769468, se.orders@cookmedical.com
Switzerland - French: +41 448009609, fr.orders@cookmedical.com
Switzerland - Italian: +41 448009609, it.orders@cookmedical.com
Switzerland - German: +41 448009609, de.orders@cookmedical.com
United Kingdom: +44 2073654183, uk.orders@cookmedical.com

USA Website: cookmedical.com
EDI: cookmedical.com/edi.do
Americas:
Phone: +1 812.339.2235, 800.457.4500, Fax: 800.554.8335
E-mail: customersupport@cookmedical.com
Australia:
Phone: +61 734346000, 1800777222, Fax: +61 734346001, 1800077283
E-mail: cau.custserv@cookmedical.com



AI, ESC, IR, OHNS, PI, RH, SUR-8.5X11