

Nester[®] | EMBOLIZATION COILS
AND MICROCOILS

Value Analysis

AND PRODUCT INFORMATION

CONTAIN COSTS

BY USING NESTER COILS
ALONE OR IN COMBINATION
WITH OTHER COILS.

2024
UPDATE



COOK[®]
MEDICAL

Disclaimer: The information provided herein reflects Cook's analysis of the procedure(s) and/or device(s), based upon the instructions for use (IFU), from sources that may include, but are not limited to, published journal articles, data on file with the manufacturer, physician and consultant input, the CPT coding system, and Medicare payment systems. This analysis is provided for general information purposes only, and Cook does not warrant or assume any liability or legal responsibility for this information. This analysis has been prepared for value analysis committees in a hospital setting. The entity assessing the product is solely responsible for determining the accurate cost of treatment at its site and the codes assigned to the services and items in the medical record. Each entity should use its own economic data to fully assess the assumptions and analysis stated herein.

Contents

- Product overview 3**
 - Product information 4
- Value analysis..... 5**
 - Overview 5
 - Economic value analysis 6
 - Nonclinical data analysis 8
 - Summary..... 9
- Materials management information..... 10**
 - Order numbers and sizing 10
 - Product specifications 11
 - Material composition 11
 - Coding and reimbursement 12
 - FDA 510(k) clearance letter 13
 - Instructions for use (IFU)..... 19
- Solutions portfolio 23**
 - Clinical**
 - Vista training and educational programs 23
 - Reimbursement 23
 - Purchasing**
 - Digital catalog 23
 - E-commerce 23
 - GS1 23
 - Customer support and distribution**
 - Distribution support 24
 - Shipping 24
 - Item master clean-up 24
 - Product use and SKU reduction 24
 - Consolidated packaging 24
 - Embolization Services..... 24
 - Sustainability 24**
- References..... 25**

Product overview

Cook Medical has manufactured embolization coils for over 35 years. Embolization coils are minimally invasive devices that are introduced percutaneously via a catheter. These devices are implantable, are supplied sterile, and are intended for one-time use.

Nester® Embolization Coils* are commonly used in interventional procedures that include permanent vessel (arterial or venous) occlusion, which are intended to treat various conditions.

Nester Embolization Coils are specifically designed with synthetic fibers that have been shown to significantly reduce the number of coils required to occlude peripheral arteries and veins.^{1,2}

Key product features:

The coils are available in a wide range of configurations	Lengths from 2 to 20 cm Diameters from 2 to 20 mm when coiled 0.018 inch and 0.035 inch platforms
Designed to form a tight occluding mass	Nester coils conform inside the vessel to create a tight occluding mass
Made of soft platinum for tight packing	Nester coils are suitable for use as starting, packing, and finishing coils
Fully fibered for thrombogenicity	The synthetic fibers promote clot formation
Easily visible under fluoroscopy	
MR conditionally safe at 3T and 1.5T	
Can be used in combination with other pushable and detachable embolization coils	

* For the purposes of this document, the reference to Nester coils includes both .035" coils and .018" microcoils.

The key considerations for your value analysis include:

1. The product

The incorporation of fibers in a metallic embolization coil design allows for the creation of a tight occluding mass,¹ which can potentially reduce the number of coils required to achieve occlusion.

2. The financial impact

Nester Embolization Coils are a potential cost-effective option for acute occlusion; they are notably less expensive than detachable coils, which means it may be less costly to treat patients.³

Product information

Product Intended Use

Nester Embolization Coils are intended for arterial and venous embolization in the peripheral vasculature.

Product design

Nester Embolization Coils are made of platinum with spaced synthetic fibers and are supplied preloaded in a loading cartridge. They are designed to be delivered to the target vessel using a soft, straight wire guide through a standard angiographic catheter. Nester coils are available in lengths from 2 cm to 20 cm and in diameters of 2 mm to 20 mm for 0.018 and 0.035 inch diameter platforms.

Deployment method

The embolization coil is loaded into the catheter by inserting the cartridge through the catheter hub until it is seated in the flare of the catheter.

The coil is then pushed into the catheter using a loading stylet or wire guide. The cartridge can then be removed, and the coil can then be pushed through the catheter shaft with a flexible tipped wire guide.

The coil is deployed when the coil and wire pass the end of the catheter tip. See the IFU for step-by-step instructions for use, coil delivery techniques, and coil size selection.



Value analysis

Overview

Using cost, quality, and clinical outcomes to make evidence-based decisions

Healthcare professionals understand the importance of a high-quality product and one that makes economic sense as well. In this ever-changing healthcare landscape, healthcare providers must not only focus on the best clinical option for their patients, but also the most cost-effective option. They can no longer focus solely on the individual procedure, but on the total care of that patient, including follow-up, return to work, and a patient’s overall quality of life.



The value analysis for the Nester Embolization Coils focuses on the variable that can be controlled—the choice of embolization coil—thus allowing healthcare providers to make evidence-based decisions to treat their patients.

Patients	Results in potentially quicker occlusion times, which can shorten the procedure, leading to conceivably less radiation exposure compared to bare metal coils based on animal study results ^{1,2}
Healthcare providers	Can be used alone or in combination with other Cook Medical or competitor coils to provide occlusion options for patients
Hospitals	Provides positive clinical outcomes and help keep costs in check by using fewer, fibered pushable coils ^{1,2,3}
Payers	Potential cost savings by reducing the number of embolization coils needed to achieve acute occlusion compared to bare metal coils ^{1,2} and by being notably less expensive than detachable coils ³

Economic value analysis

Economic value and device selection for acute vascular occlusions

Alternatives to the Nester Embolization Coils include vascular plugs and detachable coils. Vascular plugs can at times be difficult or impossible to place in tortuous arteries and therefore may make it necessary for the interventionalist to use coils. Additionally, use of a larger sheath to deliver the embolization device may result in an increased rate of access site complications.⁴ Detachable coils may be an option as well, but the total cost of detachable coils compared to pushable coils is much higher.^{4,7} The overall cost of care must be considered as part of the value analysis. In addition, animal studies suggest that less coil length is needed if the coils are fibered.^{1,2} This has cost implications when choosing between fibered and nonfibered coils. Cook Medical offers a fully fibered coil portfolio.

Detachable coils may increase the overall cost to treat the patient

The table below contains the cost data considered by Centers for Medicare & Medicaid Services (“CMS”) in finalizing CY 2024 Medicare payment rates for embolization procedures when performed in the outpatient hospital setting. The total reimbursement rate per procedure may be significantly less than the average hospital outpatient cost per procedure.

HCPCS	Description	APC	Geometric Mean Cost ^a	Payment Rate ^a
37241	Vascular embolization or occlusion, inclusive of all radiological supervision and interpretation, intraprocedural roadmapping, and imaging guidance necessary to complete the intervention; venous, other than hemorrhage (eg, congenital or acquired venous malformations, venous and capillary hemangiomas, varices, varicoceles)	5193	\$12,686.86	\$10,492.72
37242	Vascular embolization or occlusion, inclusive of all radiological supervision and interpretation, intraprocedural roadmapping, and imaging guidance necessary to complete the intervention; arterial, other than hemorrhage or tumor (eg, congenital or acquired arterial malformations, arteriovenous malformations, arteriovenous fistulas, aneurysms, pseudoaneurysms)	5194	\$15,432.58	\$16,724.70
37243	Vascular embolization or occlusion, inclusive of all radiological supervision and interpretation, intraprocedural roadmapping, and imaging guidance necessary to complete the intervention; for tumors, organ ischemia, or infarction	5193	\$12,210.54	\$10,492.72
37244	Vascular embolization or occlusion, inclusive of all radiological supervision and interpretation, intraprocedural roadmapping, and imaging guidance necessary to complete the intervention; for arterial or venous hemorrhage or lymphatic extravasation	5193	\$14,867.30	\$10,492.72

Scenarios: Costs Comparing Pushable Nester Coils and Detachable Coils

Costs per procedure	Pushable Nester Embolization Coils	Detachable Coils
Estimated number of coils per procedure ⁸	10	5
Total cost of coils per procedure ^b	\$977.50	\$3,020.10 ^b

Pushable and Detachable Coil Combination Comparisons		Pushable Nester Embolization Coils	Detachable Coils	\$ Totals
All Detachable Coils	Estimated number of coils per procedure ⁸	0	5	
	Total cost of coils per procedure ^b	0	\$3,020.10 ^b	\$3,020.10
Combination of Coils	Estimated number of coils per procedure ⁸	6	2	
	Total cost of coils per procedure ^b	\$586.50	\$1,208.04	\$1,794.54
All Pushable Coils	Estimated number of coils per procedure ⁸	10	0	
	Total cost of coils per procedure ^b	\$977.50	\$0	\$977.50

For more information on the clinical use and economic impact of Nester embolization coils, please contact your local Cook Medical Representative.


^a CY 2024 Hospital Outpatient Prospective Payment System (OPPS) and Ambulatory Surgical Center (ASC) Payment System Medicare & Medicaid Services Final Rule. Centers for Medicare & Medicaid Services. <https://www.cms.gov/medicare/payment/prospective-payment-systems/hospital-outpatient/regulations-notice/cms-1786-fc>. Accessed 15 Nov 2023.

^b The estimated cost of each Nester Embolization Coil was \$97.75 and the estimated cost of each Detachable coil was \$604.02. Coil price estimates are averages from ECRI data.

Nonclinical data analysis

Metallic coils are a mainstay of embolotherapy. Coils have evolved considerably over the past several decades with a transition of metal from stainless steel to platinum, from wool to polymer fibers (for fibered coils) and hydrogel, and with the development of detachable coils.

Nester Embolization Coils with nylon fibers allow significantly fewer embolization coils to achieve acute occlusion than Nester non-fibered coils.^{1,2} Fewer coils required can lead to a potential cost savings, shorten procedure times, leading to conceivably less radiation exposure, and lessen the amount of metal left in the body when compared to bare metal coils.^{1,2}

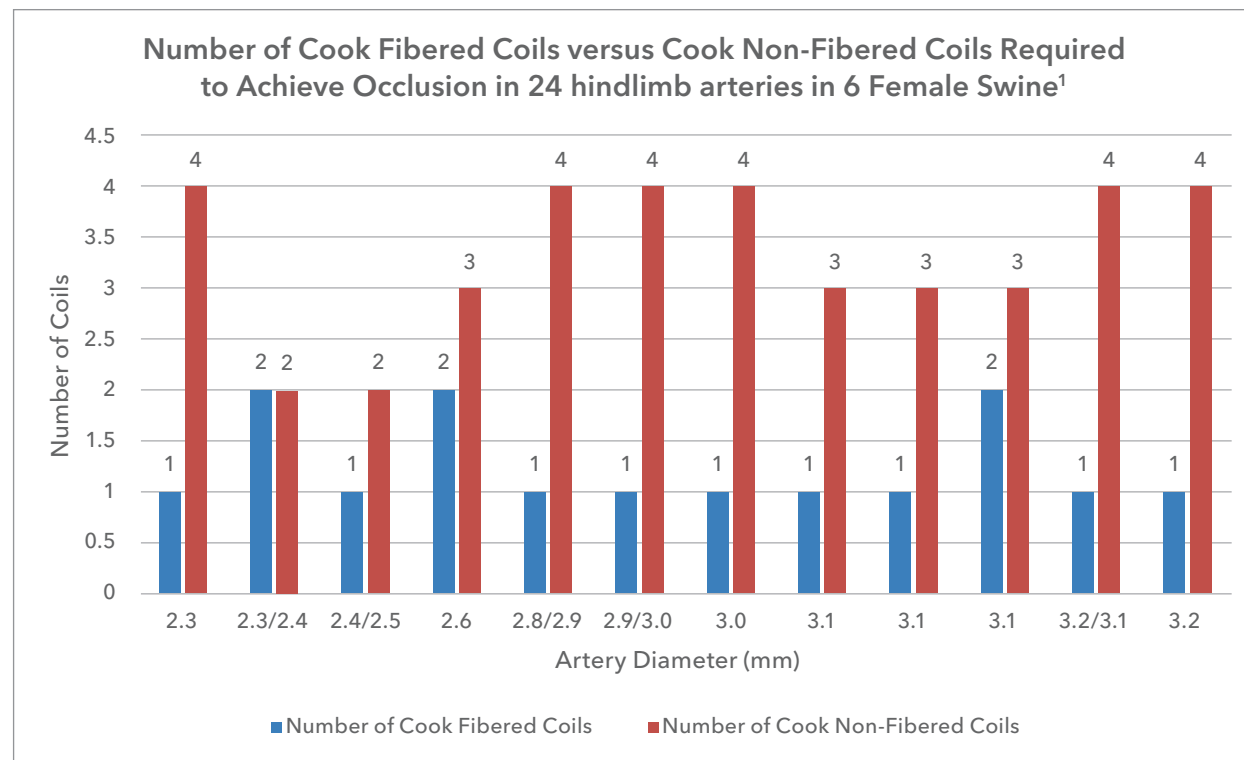

Summary

Embolization can be complicated, but embolization coil choice does not have to be. The data referenced throughout this document can help healthcare providers make evidence-based decisions. By using this information, providers can determine if Nester Embolization Coils are an ideal choice for their patients.

Nester coils are designed to provide value for:

Patients	Results in potentially quicker occlusion times, which can shorten the procedure, leading to conceivably less radiation exposure compared to bare metal coils ^{1,2}
Healthcare Providers	Can be used alone or in combination with other Cook Medical coils or competitor coils to provide occlusion options for patients
Hospitals	Provides positive clinical outcomes and keeps costs in check by using fewer, fibered pushable coils; thus it becomes potentially less costly to treat patients ^{1,2,3}
Payers	Potential cost savings by reducing the number of embolization coils needed to achieve acute occlusion compared to bare metal coils ^{1,2} and by being notably less expensive than detachable coils ³

Considerations for your value analysis include:

1. The product

The incorporation of fibers in a metallic embolization coil design allows for the creation of a tight occluding mass, which can potentially reduce the number of coils required to achieve occlusion.^{1,2}

2. The specialties served

- Vascular surgeons
- Interventional radiologists
- Interventional cardiologists

3. The financial impact

Nester Embolization Coils are a potential cost-effective option for acute occlusion since they are notably less expensive than detachable coils.³

4. The impact on patients

With a potentially quicker occlusion time and fewer coils required to achieve occlusion, patients will conceivably receive less radiation exposure with a smaller amount of metal left in the body, compared to bare metal coils.^{1,2}

Materials management information

Order numbers and sizing

Order Number	Reference Part Number	Extended Embolus Length cm	Coiled Embolus Diameter mm
0.018 inch Diameter Nester® Embolization Microcoils			
G47344	MWCE-18-2-2-NESTER-01	2	2
G47331	MWCE-18-3-2-NESTER-01	3	2
G47332	MWCE-18-3-3-NESTER-01	3	3
G47333	MWCE-18-5-2-NESTER-01	5	2
G47334	MWCE-18-5-3-NESTER-01	5	3
G47335	MWCE-18-5-5-NESTER-01	5	5
G47337	MWCE-18-7-2-NESTER-01	7	2
G47338	MWCE-18-7-3-NESTER-01	7	3
G47339	MWCE-18-7-4-NESTER-01	7	4
G47340	MWCE-18-7-5-NESTER-01	7	5
G47341	MWCE-18-7-6-NESTER-01	7	6
G47342	MWCE-18-7-8-NESTER-01	7	8
G47326	MWCE-18-14-3-NESTER-01	14	3
G47327	MWCE-18-14-4-NESTER-01	14	4
G47328	MWCE-18-14-5-NESTER-01	14	5
G47329	MWCE-18-14-6-NESTER-01	14	6
G47330	MWCE-18-14-8-NESTER-01	14	8
G47325	MWCE-18-14-10-NESTER-01	14	10

Some products or part numbers may not be available in all markets. Contact your local Cook representative or Customer Support & Distribution for details.

Order Number	Reference Part Number	Extended Embolus Length cm	Coiled Embolus Diameter mm
0.035 inch Diameter Nester® Embolization Coils			
G47371	MWCE-35-7-3-NESTER-01	7	3
G47372	MWCE-35-7-4-NESTER-01	7	4
G47374	MWCE-35-7-6-NESTER-01	7	6
G47375	MWCE-35-7-8-NESTER-01	7	8
G47365	MWCE-35-7-10-NESTER-01	7	10
G47352	MWCE-35-14-4-NESTER-01	14	4
G47354	MWCE-35-14-6-NESTER-01	14	6
G47355	MWCE-35-14-8-NESTER-01	14	8
G47345	MWCE-35-14-10-NESTER-01	14	10
G47346	MWCE-35-14-12-NESTER-01	14	12
G47347	MWCE-35-14-14-NESTER-01	14	14
G47348	MWCE-35-14-16-NESTER-01	14	16
G47349	MWCE-35-14-18-NESTER-01	14	18
G47350	MWCE-35-14-20-NESTER-01	14	20
G47356	MWCE-35-20-10-NESTER-01	20	10
G47357	MWCE-35-20-12-NESTER-01	20	12
G47358	MWCE-35-20-14-NESTER-01	20	14
G47359	MWCE-35-20-16-NESTER-01	20	16
G47360	MWCE-35-20-18-NESTER-01	20	18
G47361	MWCE-35-20-20-NESTER-01	20	20

Some products or part numbers may not be available in all markets. Contact your local Cook representative or Customer Support & Distribution for details.

If you like Nester Embolization Coils, you may also be interested in the other coils in Cook Medical's embolization portfolio, as well as Cook Medical devices that support embolization and other vascular procedures: www.cookmedical.com/products/

Product indication

Nester Embolization Coils and Microcoils are intended for arterial and venous embolization in the peripheral vasculature.

Material composition

Nester Embolization Coils are made of a platinum alloy (92% platinum, 8% tungsten) with equidistantly spaced nylon fibers between the coils and are supplied preloaded in a loading cartridge. They are designed to be delivered to the target vessel using a soft, straight wire guide through a standard angiographic catheter. Nester Embolization Coils are loaded onto an 19 or 21 gage (depending upon coil diameter) hubbed stainless steel shipping cannula. The length of the cannula is based upon the coil length. A pusher stylet is provided with the 0.018 inch diameter microcoils. The pusher is designed with a rounded ½ inch handle coiled in an offset manner for easy grip. Both ends of the pusher are rounded to a smooth finish.

Nester Embolization Coils are manufactured from platinum coiled wire and are recommended for use with PTFE-coated wire guides manufactured as a straight guide with a flexible distal tip. In addition, the deployment of platinum embolization coils is not recommended for use with polyurethane or polyvinylchloride catheters or any catheters with distal side ports since the material or sideport may result in a jamming of the embolus within the catheter.^c


Coding and reimbursement

For the most up-to-date information, please visit <https://www.cookmedical.com/support/reimbursement/>

Go to [Coding and Reimbursement Guides > Interventional Radiology > Transcatheter Peripheral Embolization or Occlusion Services.](#)

FDA 510(k) clearance letter

This document is also available at <https://www.accessdata.fda.gov/scripts/cdrh/cfdocs/cfpmn/pmn.cfm?ID=K153778>

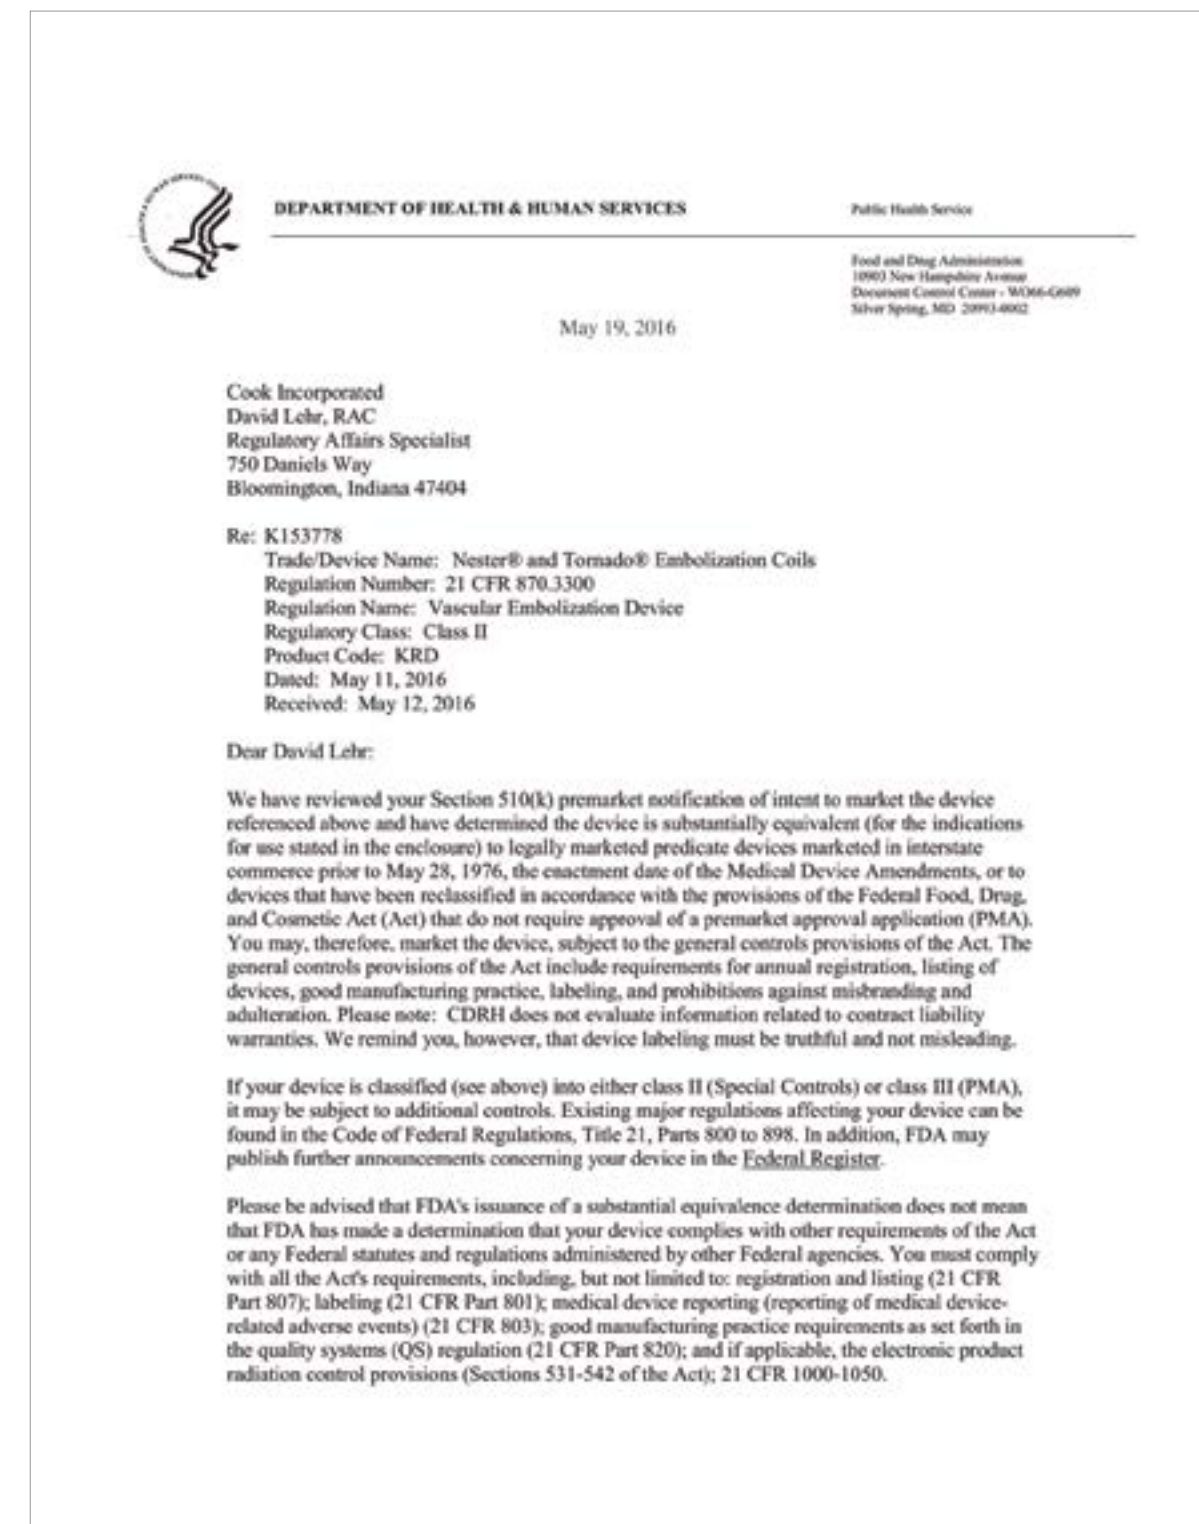

^c Data on file with manufacturer. Reference document number: Design Dossier: 016-031 (Rev. 8)

Page 2 - David Lehr

If you desire specific advice for your device on our labeling regulation (21 CFR Part 801), please contact the Division of Industry and Consumer Education at its toll-free number (800) 638-2041 or (301) 796-7100 or at its Internet address

<http://www.fda.gov/MedicalDevices/ResourcesforYou/Industry/default.htm>. Also, please note the regulation entitled, "Misbranding by reference to premarket notification" (21 CFR Part 807.97). For questions regarding the reporting of adverse events under the MDR regulation (21 CFR Part 803), please go to <http://www.fda.gov/MedicalDevices/Safety/ReportaProblem/default.htm> for the CDRH's Office of Surveillance and Biometrics/Division of Postmarket Surveillance.

You may obtain other general information on your responsibilities under the Act from the Division of Industry and Consumer Education at its toll-free number (800) 638-2041 or (301) 796-7100 or at its Internet address <http://www.fda.gov/MedicalDevices/ResourcesforYou/Industry/default.htm>.

Sincerely yours,

Kenneth J. Cavanaugh -S

for
Bram D. Zuckerman, M.D.
Director
Division of Cardiovascular Devices
Office of Device Evaluation
Center for Devices and Radiological Health

Enclosure

DEPARTMENT OF HEALTH AND HUMAN SERVICES Food and Drug Administration	Form Approved: OMB No. 0910-0120 Expiration Date: January 31, 2017 See PRA Statement below.
Indications for Use	

510(k) Number (if known)
K153778

Device Name
Nester® and Tomado® Embolization Coils

Indications for Use (Describe)
The Nester® and Tomado® Embolization Coils are intended for arterial and venous embolization in the peripheral vasculature.

Type of Use (Select one or both, as applicable)

Prescription Use (Part 21 CFR 801 Subpart D) Over-The-Counter Use (21 CFR 801 Subpart C)

CONTINUE ON A SEPARATE PAGE IF NEEDED.

This section applies only to requirements of the Paperwork Reduction Act of 1995.
"DO NOT SEND YOUR COMPLETED FORM TO THE PRA STAFF EMAIL ADDRESS BELOW."
The burden time for this collection of information is estimated to average 79 hours per response, including the time to review instructions, search existing data sources, gather and maintain the data needed and complete and review the collection of information. Send comments regarding this burden estimate or any other aspect of this information collection, including suggestions for reducing this burden, to:

Department of Health and Human Services
Food and Drug Administration
Office of Chief Information Officer
Paperwork Reduction Act (PRA) Staff
PRAStaff@fda.hhs.gov

"An agency may not conduct or sponsor, and a person is not required to respond to, a collection of information unless it displays a currently valid OMB number."



K153778

COOK INCORPORATED
750 DANIELS WAY, P.O. BOX 499
BLOOMINGTON, IN 47402-0499 U.S.A.
PHONE: 812.339.2222 FAX: 812.417.4340
WWW.COOKMEDICAL.COM

2.0 510(k) SUMMARY

As required by 21 CFR §807.92
Date Prepared: April 1, 2016

I. SUBMITTER

Submission: Traditional 510(k) Premarket Notification
Applicant: Cook Incorporated
Contact: David Lehr, RAC
Applicant Address: Cook Incorporated
750 Daniels Way
Bloomington, IN 47404
Contact Phone Number: (812) 335-3575 ext. 102309
Contact Fax Number: (812) 332-0281

II. DEVICE

Trade Name: Nester® and Tornado® Embolization Coils
Common Name: Vascular Embolization Device
Classification Name: Device, Vascular, For Promoting Embolization
Regulation/Class: 21 CFR §870.3300/Class II
Product Code: KRD

III. PREDICATE DEVICE

The device subject of this submission is considered substantially equivalent to the predicate device, the Cook Retractable® Detachable Embolization Coil (K123712/K151676). This predicate has never been subject to a design-related recall.

IV. DEVICE DESCRIPTION

The Nester® and Tornado® Embolization Coils are constructed from coiled platinum wire and synthetic fibers. The wire forms primary coil diameters that can be delivered through catheters with end hole diameters of 0.018, 0.035, and 0.038 inch. For the Nester® Embolization Coils, the extended embolus lengths range from 3 to 20 cm, and upon deployment the coiled embolus diameters range from 2 to 20 mm. For the Tornado® Embolization Coils, the extended embolus lengths range from 2 to 14.2 cm, and upon deployment the coiled embolus tapering diameters range from 3/2 to 10/5 mm.

V. INDICATIONS FOR USE

The Nester® and Tornado® Embolization Coils are intended for arterial and venous embolization in the peripheral vasculature.

Cook Incorporated – Traditional 510(k)
Nester® and Tornado® Embolization Coils
March 30, 2016

2

VI. COMPARISON OF TECHNOLOGICAL CHARACTERISTICS WITH THE PREDICATE DEVICE

The subject devices, the Nester® and Tornado® Embolization Coils, and the predicate device, the Retractable® Detachable Embolization Coil (K123712/151676), are substantially equivalent in that these devices have identical intended uses and similar technological characteristics. The predicate device is a combined embolization coil and delivery wire. Its embolization coil (made of platinum wire and nylon fibers) is delivered by a detachment mechanism. The subject devices are pushable embolization coils (also made of platinum wire and nylon fibers) delivered with a wire guide through a delivery catheter. The predicate coils (intended for delivery through catheters with an end hole size of 0.035 inch) have a helical shape, and are available in lengths of 7 cm or 14 cm and diameters ranging from 4 to 20 mm. The subject Nester coils (intended for delivery through catheters with end hole sizes of 0.018, 0.035, and 0.038 inch) also have a helical shape and are available in lengths ranging from 2 to 20 cm and in diameters ranging from 2 to 20 mm. The subject Tornado coils (also intended for delivery through catheters with end hole sizes of 0.018, 0.035, and 0.038 inch) have a tapered vortex (or tomado) shape and are available in lengths ranging from 2.0 to 14.2 cm and tapering diameters ranging from 3/2 to 10/5 mm. Additionally, the subject devices, like the predicate device, are labeled as MR Conditional. However, there are differences in the MR scanning conditions to reflect the testing performed on the subject devices. Based on the comparison of the design, intended use, materials, fundamental technology, and principle of operation, the subject devices are considered to be substantially equivalent to the currently marketed predicate device.

VII. PERFORMANCE DATA

The subject devices underwent the applicable testing listed below to ensure reliable design and performance under the testing parameters. Performance (bench, MRI, and animal) and biocompatibility testing was conducted in accordance with applicable FDA guidance documents to confirm the reliable performance of critical device characteristics.

- Biocompatibility Testing – Cytotoxicity, Sensitization, Intracutaneous Reactivity, Acute Systemic Toxicity, Subchronic Toxicity, Genotoxicity, Implantation, Hemocompatibility, and Pyrogenicity tests were performed on the implantable embolization coils. Cytotoxicity, Sensitization, Intracutaneous Reactivity, Acute Systemic Toxicity, and Hemocompatibility tests were performed on the device's

Cook Incorporated – Traditional 510(k)
Nester® and Tornado® Embolization Coils
March 30, 2016

3

loading stylet and loading cartridge. All tests results met the acceptance criteria, where applicable, or demonstrated that the device is biocompatible.

- Wire Tensile Testing – Testing shows the raw wire has a peak load value greater than or equal to the minimum tensile strength requirements. The predetermined acceptance criteria were met.
- Coil Tensile Testing – Testing characterized the embolization coils' uniaxial tensile strength.
- Rotations to Failure Testing – Testing characterized the embolization coils' torque strength.
- Delivery Friction Testing – Testing shows that the embolization coils fully deploy into the portion of the target artery in an anatomical model. The predetermined acceptance criteria were met.
- Delivery Fatigue Testing – Testing shows that the embolization coils do not have any visual defect after delivery. The predetermined acceptance criteria were met.
- Fiber Security Testing – Testing shows that an entire fiber is not released from the coils during simulated delivery conditions. The predetermined acceptance criteria were met.
- MRI Testing – MRI compatibility was assessed by evaluating magnetic field interactions (displacement force and torque), artifact, and RF-induced heating in accordance with FDA guidance titled, *Establishing Safety and Compatibility of Passive Implants in the Magnetic Resonance (MR) Environment*.
- Animal Testing – One-month, three-month, and six-month safety evaluations in swine were performed on platinum embolization coils. Testing shows that the target arteries do not indicate a substantially adverse biological response. The predetermined acceptance criteria were met.

VIII. CONCLUSIONS

The data included in this submission indicate that the subject devices do not raise new questions of safety or effectiveness compared to the predicate device. This supports a determination of substantial equivalence.

Instructions for use (IFU)*

NESTER® EMBOLIZATION COILS AND MICROCOILS

CAUTION: U.S. federal law restricts this device to sale by or on the order of a physician (or a properly licensed practitioner)

DEVICE DESCRIPTION

Nester Embolization Coils (0.035" and 0.038") and 0.018" Microcoils are made of platinum with spaced synthetic fibers, and are supplied preloaded in a loading cartridge. They are designed to be delivered to the target vessel using a soft, straight wire guide through a standard angiographic catheter.

INTENDED USE

Nester Embolization Coils and Microcoils are intended for arterial and venous embolization in the peripheral vasculature.

MRI SAFETY INFORMATION

Nonclinical testing has demonstrated that single and multiple Nester Embolization Coils and Microcoils are MR Conditional according to ASTM F2503. A patient with this device may be safely scanned after placement under the following conditions:

- Static magnetic field of 3.0 tesla or 1.5 tesla only
- Maximum magnetic field spatial gradient of 1700 gauss/cm (17 T/m) or less
- Maximum MR system reported, whole-body-averaged specific absorption rate (SAR) of ≤ 2.0 W/kg (Normal Operating Mode)

Under the scan conditions provided above, the Nester Embolization Coils and Microcoils are not expected to result in a temperature rise of more than 3.0° C after 15 minutes of continuous scanning.

The image artifact extends approximately 5.7 mm from the Nester Embolization Coils and Microcoils as found during nonclinical testing when imaged with a gradient echo pulse sequence and a 3.0 Tesla MRI system.

CONTRAINDICATIONS

None known

WARNINGS

- Positioning of Embolization Coils and Microcoils should be done with particular care. Coils should not be left too close to the inlets of arteries and should be intermeshed with previously placed coils if possible. A minimal but sufficient arterial blood flow should remain to hold the coils against the previously placed coils until a solid clot ensures permanent fixation. The purpose of these suggestions is to minimize the possibility of loose coils becoming dislodged and obstructing a normal and essential arterial channel.
- Nester Embolization Coils and Microcoils are not recommended for use with polyurethane catheters or catheters with sideports. If a catheter with sideports is used, the embolus may lodge in the sideport or pass inadvertently through it. Use of a polyurethane catheter may also result in lodging of the embolus within the catheter.
- If difficulties occur when deploying the embolization coil, withdraw the wire guide, coil and angiographic catheter simultaneously as a unit.

*The Nester Embolization Coil IFU references the 0.038 inch, 0.035 inch and 0.018 inch size coils. Please note that as of September 30, 2019, 0.038 inch diameter size Nester coils are no longer available in the US market. The 0.035 inch diameter Nester Embolization Coil and the 0.038 inch diameter MReye® Embolization Coil are possible replacement options.

PRECAUTIONS

- The product is intended for use by physicians trained and experienced in embolization techniques. Standard techniques for placement of vascular access sheaths, angiographic catheters and wire guides should be employed.
- Perform an angiogram prior to embolization to determine correct catheter position.
- Prior to introduction of the embolization coil, flush the angiographic catheter with saline.
- If using a .018 inch Nester Embolization Microcoil, ensure that the delivery catheter has an internal diameter (ID) of .018 to .025 inch.

PRODUCT RECOMMENDATIONS

The following table offers specific recommendations.

Coil Size Diameter	Catheter Type & Size	Wire Guide Type & Size
.018 inch	MCS-2.5 MCS-2.8	STF-18 TSF-18 TSFB-18
.035 inch	HNB4.0-35 HNB4.1-35 HNB[R]5.0-35 SCBR4.0-35 SCBR5.0-35	TSF-35 TSFB-35 TSFBP-35 TSFNA-35 TSFNB-35
.038 inch	HNB[R]5.0-38 HNB[R]6.0-38 SCBR4.0-38 SCBR5.0-38	TSF-38 TSFB-38 TSFNA-38 TSFNB-38

Coil Delivery Technique and Coil Size Selection

Long-term occlusion depends on achieving cross-sectional occlusion of the blood vessel, and coaxial catheters provide the ability to control placement of coils and permanent occlusion. The combination of the coaxial technique and either the anchor or scaffold technique significantly enhances stability of coil deployment.

- Coaxial technique: The use of an outer guiding sheath/catheter is the most important step in preventing coil elongation and uncertain long-term occlusion. The outer guiding sheath/catheter provides support, and the inner catheter provides finer selective maneuvers. (Fig. 7)
- Anchor technique: The anchor technique provides safe and distal occlusion when there is a question about instability of coils. At least 2 cm of a coil is advanced into the side branch, which is normally sacrificed. The rest of the coil is then deployed just proximal to that side branch, and additional coils are packed. (Fig. 8) NOTE: Use a coil longer than 10 cm for anchor technique.
- Scaffold technique: The scaffold technique is used for high-flow vessels when there is concern about migration of a softer coil. A high radial force coil is placed initially. Then, several Inconel coils or platinum coils (soft coils) may be packed within the scaffold. (Fig. 9)

In general, the first coil selected should have a diameter that is 20% larger, or at least 2 mm oversized, than the vessel that is being occluded.

INSTRUCTIONS FOR USE

For .018 Inch Microcoils:

1. Perform an angiogram prior to embolization to determine optimal catheter position.
2. Push the loading cartridge completely into the delivery catheter. (Fig. 1)
3. Advance the Luer lock connector fitting toward the catheter hub and lock into place. (Fig. 2)
4. Use the pusher stylet to load the Nester Embolization Microcoil into the delivery catheter. (Fig. 3) NOTE: The stylet must be pushed as far as possible into the loading cartridge to ensure proper loading. Remove the pusher stylet and loading cartridge.
5. To obtain secure placement of the Nester Embolization Microcoil, we recommend the use of the pusher stylet to push the Microcoil further into the delivery catheter. (Fig. 4)
6. Once coil is positioned into delivery catheter, verify position of catheter tip prior to deployment. Coil design permits delivery into the target vessel by saline/contrast flush or by push technique using an appropriately sized wire guide or pusher.
7. Perform final angiogram to confirm coil position within target vessel.

For .035 and .038 Inch Coils:

1. Perform an angiogram prior to embolization to determine optimal catheter position.
2. Firmly grasp the loading cartridge between thumb and forefinger. Introduce the metal end of the loading cartridge into the base of the catheter hub. Lock loading cartridge onto catheter hub by turning Luer lock adapter clockwise. (Fig. 5)

3. Maintaining position of the cartridge, advance the stiff portion of the wire guide into the loading cannula. Push the coil into the first 20 to 30 centimeters of the angiographic catheter. (Fig. 6) Remove the wire guide and loading cartridge.
4. With the flexible tip of the wire guide, advance the embolization coil to the tip of the catheter. Verify position of the angiographic catheter prior to deployment.
5. Deploy the coil by advancing the wire guide past the tip of the catheter.
6. Perform final angiogram to confirm coil position within target vessel.

HOW SUPPLIED

Supplied sterilized by ethylene oxide gas in peel-open packages. Intended for one-time use. Sterile if package is unopened or undamaged. Do not use the product if there is doubt as to whether the product is sterile. Store in a dark, dry, cool place. Avoid extended exposure to light. Upon removal from package, inspect the product to ensure no damage has occurred.

REFERENCES

These instructions for use are based on experience from physicians and (or) their published literature. Refer to your local Cook sales representative for information on available literature

Figure 1.



Figure 2.



Figure 3.



Figure 4.



Figure 5.



Figure 6.



Figure 7.

Coaxial Technique to Prevent Coil Elongation

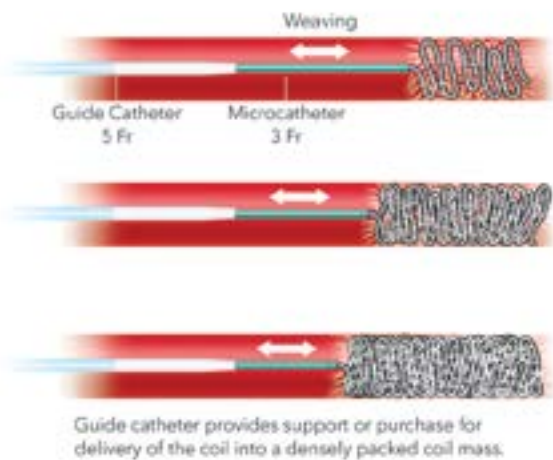


Figure 8.

Anchor Technique


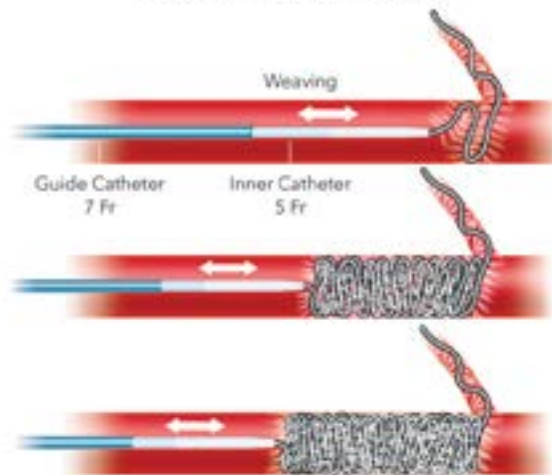


Figure 9.

Scaffold Technique

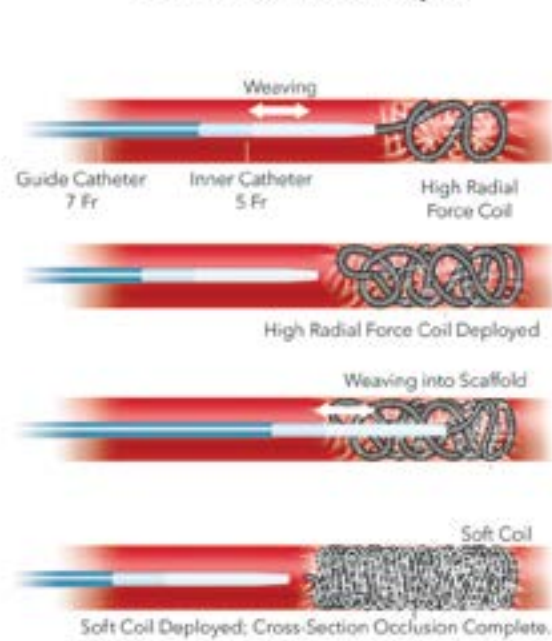

Solutions portfolio

Clinical

Vista® training and educational programs

Cook Medical's Vista training and educational programs set a high standard for product education via peer-to-peer interaction. These programs incorporate Cook-selected qualified faculty with Cook-specific content training and peer-to-peer interaction in every session. These programs are designed to focus on product education.

Visit vista.cookmedical.com for more information, or speak to your local Cook sales representative for upcoming events in your area.

Reimbursement

Cook's policy is to offer information that is complete, accurate, straightforward, and consistent with the statutes and regulations of the federal government and well-accepted coding guidelines as established by the Centers for Medicare and Medicaid Services (CMS), the American Medical Association (AMA), the American Hospital Association (AHA), and other relevant professional societies. Cook's reimbursement assistance team can provide Medicare reimbursement rates, assessment of Medicare and commercial insurance coverage policies, and coverage appeals support. Visit cookmedical.com/support/reimbursement/ for more information.

Purchasing

Digital catalog

Cook can provide a URL to an image for each product in the Cook Medical catalog. These URLs are delivered to a customer in a spreadsheet that can be uploaded to display the images in customer's purchasing platform (ERP) or clinical information system. Product images allow end users to view and validate the items.

Digital ordering

We have the ability to help you order electronically. E-commerce is an automated, paper-free method of transacting purchase orders, acknowledgments, invoices, and dispatch and receiving notifications. Cook offers value-added-network (VAN), direct EDI, XML, and web-based methods of e-commerce transactions and ordering.

GS1

GS1 is an international, not-for-profit association that creates and implements standards to bring efficiency and visibility to supply chains across multiple industries. The GS1 standards for healthcare focus on improving patient safety and supply-chain efficiency. They do this by providing unique product identification (GTINs), clean data (GDSN), and location information (GLNs) numbers.

All Cook Medical products are GS1 compliant. Having GS1-compliant products gives systems improved visibility in the supply chain.

Customer support and distribution

Distribution support

At Cook Medical, we partner with health systems to identify the distribution model that best fits their needs. We're glad to engage in a discussion regarding the desire to ship Cook Medical items through a third-party distributor or customer's self-distribution center.

Shipping

Standard shipping is included for most orders, although Cook Medical may require a minimum order quantity or dollar amount. Expedited shipping may be available and subject to an additional cost which will be prepaid by Cook Medical and invoiced to the customer. Cook Medical's shipping policy is subject to change and may be updated from time to time. Please refer to <https://www.cookmedical.com/support/ordering-returns/> for current order requirements and further information about shipping options.

Item master clean-up

Cook Medical can perform an item master clean-up for its customers. This includes, but is not limited to, helping customers correct pricing discrepancies, discover unit of measure discrepancies, locate unavailable or invalid part numbers, provide GTINs, and offer contract information. This will ensure that the ordering process between the customer and Cook Medical is seamless.

Product use and SKU reduction

Cook Medical can provide cross-referencing to all customers who request it. This includes cross-referencing between a competitor and Cook Medical and between Cook Medical's stock and nonstock items.

Consolidated packaging

Cook Medical's consolidated packaging program combines separate product orders in clear, heat-sealed plastic bags that will ensure that the integrity of each purchase order (PO) is maintained. A packing slip with scannable barcode is included in each heat-sealed pack. Our process includes placing individually bagged POs into as few boxes as possible by using a mutually agreed-upon order cutoff time. Fewer boxes received means a more streamlined receiving process, reduced shipping and freight costs, and reduced cardboard recycling waste and expense.

Embolization Services

- Personalized and customized attention
- Sales representatives that can offer case and product support when requested
- Devices for access, navigation, and treatment that support embolization procedures from start to finish
- Patient specific solutions
- Fulfillment options and business solutions assistance

Sustainability

At Cook Medical, we strive to perform in an environmentally responsible manner by incorporating the best management practices, fostering the sustainable use of natural resources, promoting pollution prevention, reducing waste generation, and recycling and reusing materials where possible within our operations. Cook Medical has a corporate sustainability team responsible for finding new ways to reduce waste for our customers and for us. Currently, our sustainability strategy is focused mainly on improving the environmental performance of our facilities, packaging, and recycling.

References

1. Trerotola SO, Pressler GA, Premanandan C. Nylon fibered versus non-fibered embolization coils: comparison in a swine model. *J Vasc Intervent Radiol*. 2019;30(6):949-955.
2. White SB, Wissing ER, Van Alstine WG, et al. Comparison of Fibered versus Nonfibered Coils for Venous Embolization in an Ovine Model. *Journal of Vascular and Interventional Radiology*. 2023;34(5):888-895.
3. Park S, Lee SJ, Lee M, et. al. Prospective randomized trial comparing pushable coil and detachable coil during percutaneous implantation of port-catheter system for hepatic artery infusion chemotherapy. *Abdom Imaging*. 2015;40(3):595-600.
4. Ryer EJ, Garvin RP, Webb TP, et al. Comparison of outcomes with coils versus vascular plug embolization of the internal iliac artery for endovascular aortoiliac aneurysm repair. *J Vasc Surg*. 2012;56(5):1239-1245.
5. Stecker MS, Fan CM, Dabydeen D. Can detachable embolization coils decrease the cost of materials for portal vein embolization procedures? *Austin J Radiol*. 2016;3(3):1051. ISSN:2473-0637.
6. Medicare Calendar Year 2024 Hospital Outpatient Prospective Payment System (OPPS) and Ambulatory Surgical Center (ASC) Payment System Medicare & Medicaid Services Final Rule. Centers for Medicare & Medicaid Services. [cms.gov/medicare/payment/prospective-payment-systems/hospital-outpatient/regulations-notices/cms-1786-fc](https://www.cms.gov/medicare/payment/prospective-payment-systems/hospital-outpatient/regulations-notices/cms-1786-fc) Accessed 15 Nov 2023.
7. Chen X. Market Insights - Transcatheter Embolization and Occlusion Devices: United States, 2023. Clarivate. Published December 2022.
8. Global Data 2022. Cardiovascular Devices, Vascular Embolization Plugs and Coils 2015-2030. Medical IC.

Additional References

Bilreiro C, Donato P, Costa JF, et. al. Varicocele embolization with glue and coils: a single center experience. *Diagn Interv Imaging*. 2017;98(7-8):529-534.

Kayssi A, Oreopoulos G, Tan KT, et. al. Combined coil embolization and foam sclerotherapy for the management of varicose veins. *Ann Vasc Surg*. 2017;38:293-297.

Libicher M, Pavlidis D, Bangard C, et. al. Occlusion of the internal iliac artery prior EVAR: comparison of coils and plugs. *Vasc Endovascular Surg*. 2012;46(1):34-39.

Masada T, Tanaka T, Sakaguchi H, et. al. Coils versus gelatin particles with or without intraarterial antibiotics for partial splenic embolization: a comparative evaluation. *J Vasc Interv Radiol*. 2014;25(6):852-858.

Stein EJ, Chittams JL, Miller M, et al. Persistence in coil-embolized pulmonary arteriovenous malformations with feeding artery diameters of 3 mm or less: a retrospective single-center observational study. *J Vasc Interv Radiol*. 2017;28(3):442-449.

Contrella BN, Sabri SS, Tracci MC, et al. Outcomes of coverage of the left subclavian artery during endovascular repair of the thoracic aorta. *J Vasc Interv Radiol*. 2015;26(11): 1609-1614.

Martin JL, Faughnan ME, Prabhudesai V. Antithrombotic use predicts recanalization of embolized pulmonary arteriovenous malformations in hereditary hemorrhagic telangiectasia. *Can Assoc Radiol J*. 2017;68(4):463-467.

Nester® Embolization Coils and Microcoils

CAUTION: U.S. federal law restricts this device to sale by or on the order of a physician (or a properly licensed practitioner).

INTENDED USE: Nester Embolization Coils and Microcoils are intended for arterial and venous embolization in the peripheral vasculature.

CONTRAINDICATIONS: None known.

WARNINGS: Positioning of Embolization Coils and Microcoils should be done with particular care. Coils should not be left too close to the inlets of arteries and should be intermeshed with previously placed coils if possible. A minimal but sufficient arterial blood flow should remain to hold the coils against the previously placed coils until a solid clot ensures permanent fixation. The purpose of these suggestions is to minimize the possibility of loose coils becoming dislodged and obstructing a normal and essential arterial

channel. • Nester Embolization Coils and Microcoils are not recommended for use with polyurethane catheters or catheters with sideports. If a catheter with sideports is used, the embolus may lodge in the sideport or pass inadvertently through it. Use of a polyurethane catheter may also result in lodging of the embolus within the catheter. • If difficulties occur when deploying the embolization coil, withdraw the wire guide, coil and angiographic catheter simultaneously as a unit.

PRECAUTIONS: The product is intended for use by physicians trained and experienced in embolization techniques. Standard techniques for placement of vascular access sheaths, angiographic catheters and wire guides should be employed. • Perform an angiogram prior to embolization to determine correct catheter position. • Prior to introduction of the embolization coil, flush the angiographic catheter with saline. • **If using a .018 inch Nester Embolization Microcoil, ensure that the delivery catheter has an internal diameter (ID) of .018 to .025 inch.**

See instructions for use for full product information.